

# Minimize Noise Figure Uncertainties

## Select From Three Flexible Solutions That Cover a Wide Range of Needs

Noise figure is often the key to characterizing a receiver and its ability to detect weak incoming signals in the presence of self-generated noise. The process of reducing noise figure begins with a solid understanding of the uncertainties in your components, subsystems and test setups. Quantifying those unknowns depends on flexible tools that provide accurate, reliable results.

Keysight's noise figure solution set – instruments, applications and accessories – helps you optimize test setups and identify unwanted sources of noise. We've been providing noise-figure test solutions for more than 50 years, beginning with basic noise meters and evolving into modern solutions based on spectrum, network, and noise-figure analyzers.

This technical overview begins with a brief noise figure primer on pages 3 through 11. Pages 12 through 19 present our current product lineup and will help you find the best solution for your application – whether you're designing for good, better or best performance in your device.

A list of related resources is included on page 20. Our series of seven application notes can help you develop a deeper understanding of noise figure and its inherent challenges.

Find out more [www.keysight.com/find/noisefigure](http://www.keysight.com/find/noisefigure)

## Noise Figure Overview

Noise figure is one of the key parameters used to characterize the ability of receivers and their lower-level components to process weak signals in the presence of thermal noise. For example, when measuring low-noise amplifiers (LNAs), noise figure describes the signal-to-noise degradation that occurs due to the internally-generated noise of the active devices within an LNA.

Accurate measurements of noise figure are crucial in product design and development. Highly accurate measurements allow for better agreement between simulations and measurements, and may help uncover noise contributors that were not considered in the simulation. Before selecting the most appropriate instrument for your application, it is important to understand two key topics: how noise figure measurements are made and the uncertainties inherent in those measurements. Noise figure measurement uncertainty depends not only on the test equipment, but is also a function of the characteristics of the device under test (DUT)—for example, S-parameters and noise parameters.

There are two main methods in use today to measure noise figure. The most prevalent method is called the Y-factor or hot/cold-source technique. It uses a noise source placed at the input of the DUT, providing two levels of input noise. This method yields noise figure and scalar gain of the DUT, and is used with both spectrum and noise figure analyzer solutions. The Y-factor technique is easy to use, and it provides good measurement accuracy, especially when the noise source has a good source match and can be connected directly to the DUT.

The other method used is called the cold-source or direct-noise method. Instead of using a noise source at the DUT's input, only a known termination (usually 50  $\Omega$ ) is needed. However, the cold-source method requires an independent measurement of the DUT's gain. This method works well with vector network analyzers, because vector error correction can be used to produce very accurate gain (S21) measurements. When using the PNA-X signal analyzer, the combination of vector error correction and the PNA-X's unique source-correction method provides the highest noise figure measurement accuracy in the industry. The other advantage of the cold-source method is that both S-parameter and noise figure measurements can be made with a single connection to the DUT. During system calibration, a noise source is required.



### Two methods are commonly used to measure noise figure

- Y-factor
- Cold-source

To find out more about these methods see Application Note (AN 57-1), Fundamentals of RF and Microwave Noise Figure Measurements, literature number 5952-8255E.

# Measurement Uncertainty

Several factors contribute to overall noise figure measurement uncertainty. When selecting a noise figure solution, it is important to choose the method that minimizes the main contributor to overall noise figure uncertainty.

Some of these contributions can be found on instrument data sheets – instrument uncertainty, excess noise ratio (ENR), and jitter. Others depend upon the interaction of the test system and the DUT. For example, there are two sources of error due to imperfect system source match (a deviation from the ideal 50 Ω). The first is mismatch error, which results from non-ideal power transfer between the test system and the DUT. The second source of error is from the interaction between the noise generated within the DUT and the source match ( $\Gamma_s$ ) seen by the DUT. Figure 1 compares the noise figure measurement uncertainties produced by the Y-factor and cold-source methods. The example amplifier has a noise figure of 3 dB, gain of 15 dB, input and output match of 10 dB, and moderate noise parameters ( $F_{min} = 2.8$  dB,  $\Gamma_{opt} = 0.27 + j0$ ,  $R_n = 37.4$ ). For the Y-factor method, the uncertainty is calculated in two different ways: with the noise source connected directly to the DUT, and with an electrical network simulating the switches and cables from an automated-test-equipment (ATE) setup placed between the noise source and the DUT (with loss correction). The PNA-X example includes the ATE network.

## Uncertainty breakdown

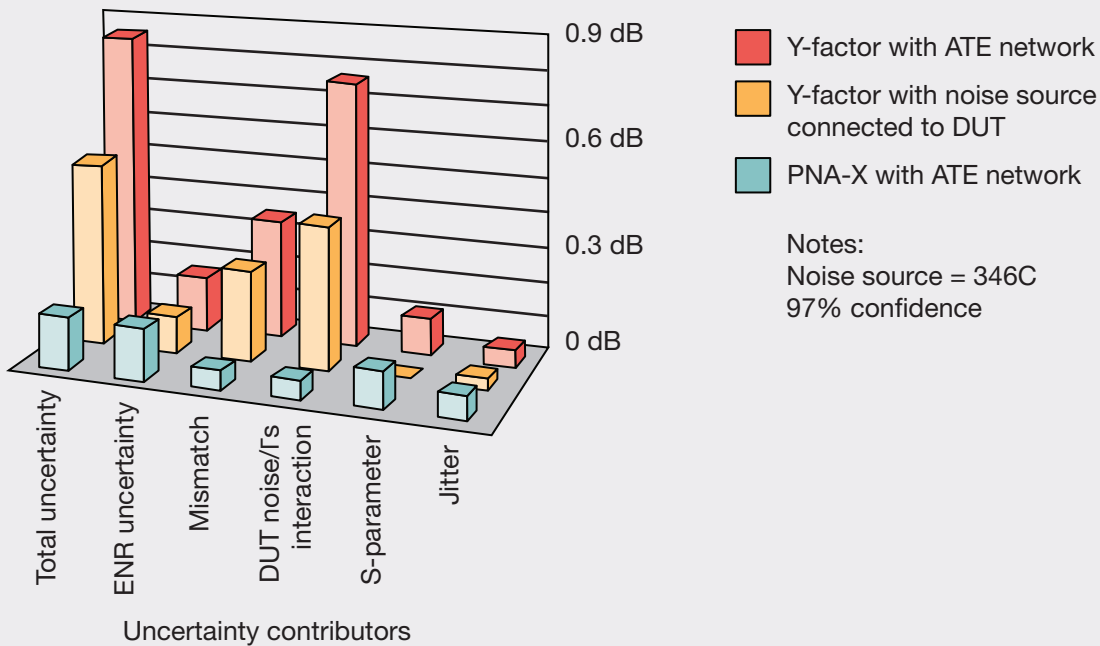


Figure 1. Breakdown of the major contributors to noise figure measurement uncertainty for the Y-factor and cold-source (with source correction) techniques.

With the Y-factor method, there are two main sources of error: mismatch between the noise source and the DUT, and the interaction of the noise generated by the DUT and the system. The simulated ATE network (inserted between the noise source and DUT) causes the errors to increase. For the PNA-X's source-corrected cold-source method, the largest source of error is the ENR uncertainty of the noise source, which affects the measurement of the PNA-X's internal noise receivers during calibration.

## DUT uncertainty

Y-factor measurement accuracy is excellent when low-ENR noise sources, such as the N4000A or 346A, can be used, and when the noise source can be connected directly to the DUT. For many devices, this scenario provides cost-effective and accurate noise figure measurements. However, measurement uncertainty usually increases if these conditions cannot be met. The PNA-X uses more advanced error-correction methods that provide excellent accuracy in all cases, and are especially useful for in-fixture, on-wafer, or automated-test environments, where Y-factor measurement uncertainty is often significantly higher. The PNA-X is also useful when additional measurements are required, such as S-parameter, compression, and intermodulation-distortion.

When the DUT is well matched and relatively insensitive to imperfect source match (deviation from the ideal 50  $\Omega$ ), then measurement uncertainty is dominated by the data-sheet specifications. In other instances, such as when measuring poorly matched devices, or when using wafer probes, imperfect system source match generates two additional sources of error that can be quite large. The first is mismatch error, which results from reflected noise power that is re-reflected by the test system, causing ripples in the measurement. The second source of error is from the interaction between the noise generated within the DUT and the source match ( $\Gamma_s$ ) presented to the DUT.

## System Components for Noise Figure Measurements

Total or overall noise figure of a system is a result of three individual components: the instrument used to measure noise figure, the noise source used in measurements or calibration, and the DUT. The Y-factor method is the basis of most noise figure measurements. It uses a noise source to determine the internal noise in the DUT while calibrating and when making measurements. In contrast, the cold-source method uses the noise source during calibration only, as shown in Figure 2.

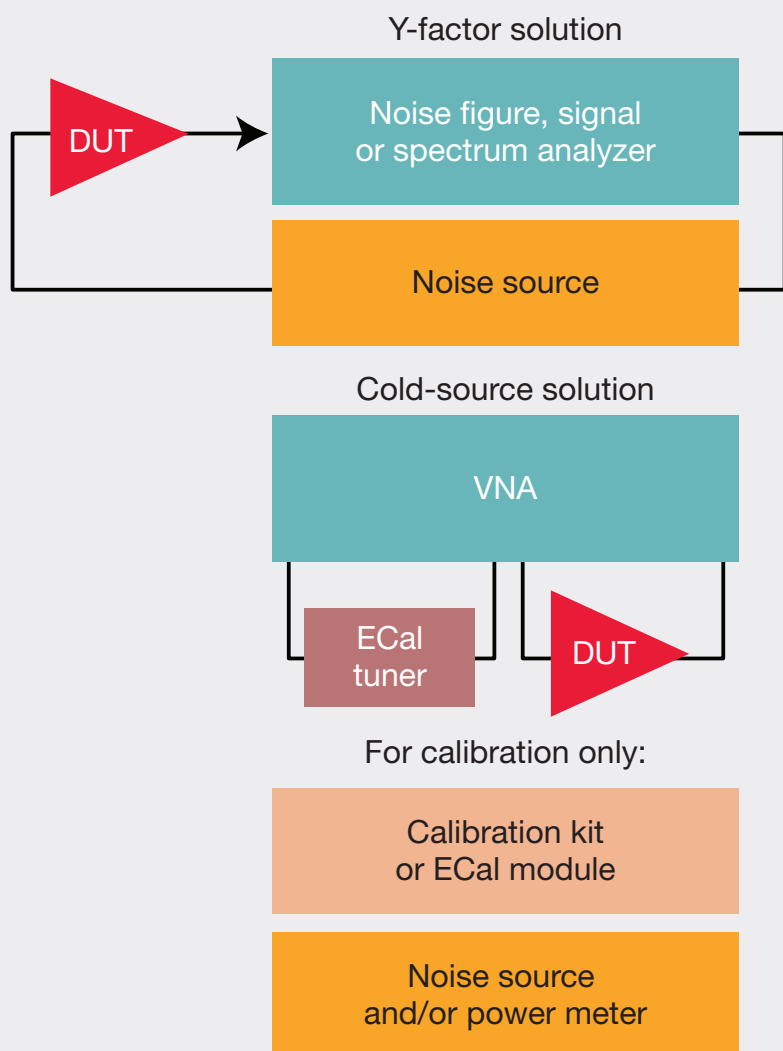


Figure 2. Basic components needed to make noise figure measurements.

Each of the components shown in Figure 2 are described in greater detail in the following sections. The Y-factor method uses either a noise figure analyzer (NFA) or a signal/spectrum analyzer with an optional noise figure measurement application. The cold-source technique uses the PNA-X network analyzer with a noise figure option to make noise figure measurements.

## Selecting an instrument

With the wide range of instruments Keysight offers for noise figure, it should be easy to find a solution that fits your requirements. Keysight offers three types of solution platforms: a dedicated noise figure analyzer, signal/spectrum analyzers, and vector network analyzers. The benefits of each are outlined below.

### Noise figure analyzer (NFA)

The NFA Series is made exclusively for accurate noise figure measurements, and uses the Y-factor method. The analyzer includes the following standard options; precision frequency reference, internal preamplifier, fine step attenuator, noise floor extension, 25 MHz analysis bandwidth, U7227A, C, or F USB external preamplifier, and a convenient snap on pouch to hold accessory items. Four model numbers covering frequency ranges 3.6, 7, 26.5, and 40 GHz that can be extended to 110 GHz with a block downconverter. The series offers low instrument noise figure, full featured signal analyzer and IQ Analyzer (Basic) modes extend beyond a dedicated noise figure analyzer.

### Signal/spectrum analyzers

Adding an optional noise figure measurement application to a versatile signal or spectrum analyzer is an economical way to add noise figure capabilities. The accuracy and frequency range of this solution depends on which base instrument it is installed. Signal/spectrum analyzers use the Y-factor method to measure noise figure. Preamplification, either external or internal, often improves accuracy.

### Network analyzers

If you need noise figure measurements with the highest accuracy, choose Keysight's PNA-X network analyzer with the noise figure option. This solution is based on the cold-source technique, and it allows S-parameter and noise figure measurements with a single connection to the DUT.

When selecting an instrument to meet your needs, it is first important to select one that will cover the frequency range of your DUT. Table 1 shows all of Keysight's noise figure solutions and the frequency ranges at which you can expect hard or nominal specifications, and where certain instruments are not recommended for noise figure measurements.



#### Keysight offers three solutions for noise figure measurements

- Noise figure analyzer – More than a dedicated noise figure analyzer with spectrum analyzer and IQ Analyzer (Basic) modes in the standard instrument.
- Signal/spectrum analyzers – economic solution with good performance
- Network analyzers – highest measurement accuracy

## Specified frequency range for noise figure performance

Instrument series	200 kHz to 10 MHz	10 MHz to 3.6 GHz	3.6 to 7 GHz	7 to 26.5 GHz	26.5 to 110 GHz
CXA					
MXA					
EXA					To 44 GHz
NFA X-Series					To 40 GHz
PXA					To 50 GHz
PNA-X					

Nominal specifications	Not recommended	Hard specifications	Nominal specifications with block downconverters
------------------------	-----------------	---------------------	--

**Table 1.** Keysight offers a wide range of instruments to cover different frequency ranges for noise figure measurements: nominal specifications are specifications based on the testing of an instrument, but are not guaranteed performance; hard specifications are specifications that are proven and guaranteed performance; and actual performance may exceed the numbers listed in the specification guide.

Measurement specifications are equally important when selecting an instrument to meet your noise figure needs. Please note that Table 2 gives the nominal specifications at 1 GHz for each instrument to enable quick, relevant comparisons. Refer to the individual specifications guide for each product for full specification information, including but not limited to hard specifications vs. nominal specifications at different frequency ranges.

## Nominal specifications at 1 GHz

Y-factor instruments	Noise figure instrument uncertainty (dB)	Noise figure gain uncertainty (dB)	Instrument match	Noise figure of the instrument (dB)
CXA	0.05	0.2	1.5	10.2
EXA	0.03	0.15	1.3	13
MXA	0.02	0.1	1.3	9.5
PXA	0.02	0.07	1.3	9.75
NFA X-Series	0.03	0.15	1.3	5.5
Cold-source instruments	Linearity	S21 parameter uncertainty	Instrument match	Noise figure of the instrument (dB)
PNA-X	0.05	0.05	1.02	12

**Table 2.** This chart compares the different noise figure solutions at 1 GHz with nominal specifications only; for full specifications, including hard specifications, please refer to the specification guide for each instrument.

## Selecting a noise source

When measuring noise figure, the quality of the noise source affects the accuracy and repeatability of your measurements. The ENRs of Keysight noise sources are carefully calibrated with traceability to national standards institutes in the U.S. and U.K. The output of a noise source is defined in terms of its frequency range and ENR. Nominal ENR values of 6 dB and 15 dB are commonly available. A low-ENR noise source will minimize error due to noise detector nonlinearity. This error will be smaller if the measurement is made over a smaller, and therefore more linear, range of the instrument's detector. A 6 dB noise source uses a smaller detector range than a 15 dB noise source.

Use a 6 dB noise source when:

- Measuring a device with gain that is especially sensitive to changes in the source impedance
- The DUT has a very low noise figure
- The device noise figure does not exceed 15 dB

Use a 15 dB noise source when:

- General-purpose applications to measure noise figure up to 30 dB
- User-calibrating the fullest dynamic range of an instrument before measuring high gain devices

Keysight offers three families of noise sources, each offering different frequency ranges, source matches, ENR, and connector types. The Smart Noise Source Series simplifies measurement setup by automatically downloading electronically stored calibration data to the instrument, saving valuable engineering time. The traditional 346 Series is the most cost-effective solution—these noise sources offer the widest range of frequency coverage. Lastly, Keysight offers high-frequency noise sources with waveguide interfaces for making measurements above 26.5 GHz. The noise source families above work with different instruments, summarized in Table 4.



## Keysight noise sources

	Noise source	ENR	Frequency range
Smart noise sources SNS Series	N4000A	4.6 to 6.5 dB	10 MHz to 198 GHz
	N4001A	14 to 16 dB	10 MHz to 18 GHz
	N4002A	12 to 17 dB	10 MHz to 26 GHz
Traditional noise sources 346 Series	346A	5 to 7 dB	10 MHz to 18 GHz
	346B	14 to 16 dB	10 MHz to 18 GHz
	346C	12 to 17 dB	10 MHz to 26 GHz
	346CK01	21 dB	1 to 50 GHz
	346CK40 <sup>1</sup>	8 db	1 to 40 GHz
High frequency noise sources 347 Series	Q347B	6 to 13 dB	33 to 50 GHz
	R347B	10 to 13 dB	26.5 to 40 GHz

1. 346CK40 ships with the N8976B.

**Table 3. Keysight offers three different families of noise sources to fit within a variety of budgets and test requirements.**

## Noise source support

Y-factor instruments	346 Series	347 Series	N4000A SNS Series
CXA	•	•	•
EXA	•	•	•
MXA	•	•	•
PXA	•	•	•
NFA X-Series	•	•	•
PNA-X	•		

**Table 4. This table lists noise source and instrument compatibility for noise figure measurements.**

# Device Under Test (DUT)

Your DUT contributes to the overall noise figure uncertainty based on its individual noise figure, gain, port match, and noise parameters. In general, there are two scenarios to consider when choosing the Y-factor method. When the output noise of the DUT is well above the input noise of the analyzer, the analyzer with the best instrument uncertainty gives the most accurate results, and the MXA signal analyzer is the best choice. If the output noise of the DUT is smaller, select the NFA noise figure analyzer, which gives the lowest uncertainty. Refer to Table 2 to compare the nominal specifications of these solutions at 1 GHz.

Figure 3 shows how DUT gain affects noise figure uncertainty when using a spectrum analyzer or noise figure analyzer. This example is at 1 GHz with a 346A noise source and assumes the DUT has a 1.5 dB noise figure and 1.5:1 VSWR.

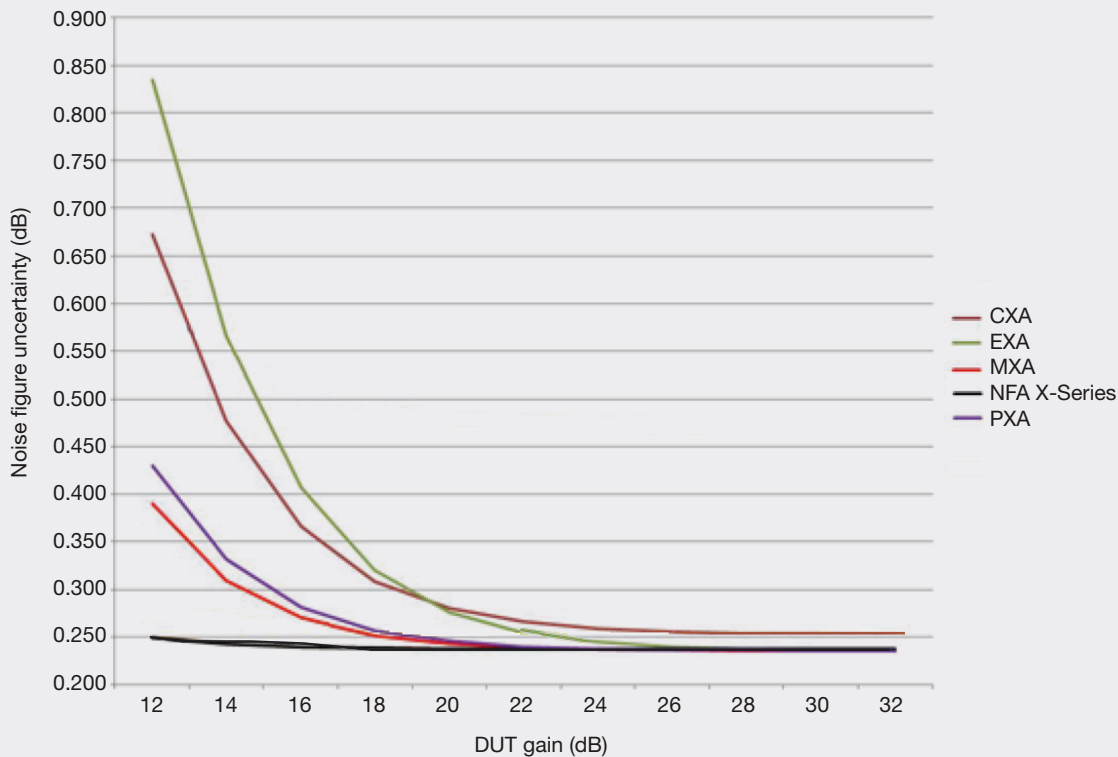


Figure 3. As the gain of a DUT decreases, Y-factor noise figure measurement uncertainty increases; below 20 dB of gain, there are significant differences between the various instrument choices.

The values in Figure 3 were computed with the noise figure uncertainty calculator and the nominal specifications at 1 GHz shown in Table 2. The uncertainty calculator can be found at [www.keysight.com/find/nfu](http://www.keysight.com/find/nfu). The uncertainty calculator can be used for either of the following cases:

### Modeling the performance of your system

For this purpose, defaults are available for Keysight's noise figure instruments and noise sources. These defaults have typical values associated with them and can be useful for estimating the effect individual parameters have in overall uncertainty levels.

### Making actual calculations of the uncertainty of your system

You will need to obtain accurate values of all the associated parameters in question, such as match and gain. Please consult the calibration certificates of your instruments to obtain their measured uncertainty parameters.

# The Only Dedicated Noise Figure Analyzer on the Market



## Noise figure analyzer (NFA)

- N8973B
- N8974B
- N8975B
- N8976B

The NFA X-Series are much more than dedicated noise figure analyzers. Further analyze DUT anomalies using full featured spectrum analysis and IQ Analyzer (Basic) modes on the standard analyzer. Ease of use features allow any engineer or technician to quickly setup measurements correctly, view those measurements in different formats, and either print the results or save them. The Multiple DUT Setup and Calibration feature allows a user to cal and measure up to 12 different DUT setups. View all 7 noise figure related parameters using Table View. Use the Signal Path Configurator interactive tool to help you optimize your measurements for the lowest possible uncertainties. Repeatable, reliable measurements provide results that you can trust. As a result, you will be able to produce more robust designs and prototypes in the lab, and achieve higher yields and throughput in manufacturing.

## Features

- Fours models; 3.6, 7, 26.5, and 40 GHz with extension to 110 GHz wit block downconverters
- Fully specified to 40 GHz with precision frequency reference, internal preamplifier, fine step attenuator, noise floor extension, 25 MHz analysis BW, USB external preamplifier, snap on accessory pouch.
- Works with Keysight SNS series noise sources, 346 and 347 series noise sources
- Built-in interactive uncertainty calculator
- Multiple DUT Setup and Calibration
- (7) noise figure metrics displayed at once using Table View
- Signal Path Configurator

## Literature resources

- NFA Series Noise Figure Analyzers Data Sheet, literature number 5992-1270EN

# Noise Figure for Keysight's Fastest Signal Analyzers



## X-Series signal analyzers

- N9030B PXA
- N9020/21B MXA
- N9010B EXA
- N9000B CXA

Keysight's X-Series noise figure measurement application offers development engineers a simple tool to make accurate and repeatable measurements. The noise figure option utilizes the easy user interface and incredible speed of the Keysight X-Series signal analyzers. The built-in help and internal step-by-step diagrams allow new users to start making measurements instantly and save their results quickly. The W9069C for the CXA signal analyzer offers hard specification up to 26.5 GHz. The N9069C pairs with the EXA for hard specifications up to 44 GHz; MXA and PXA for hard specifications up to 50 GHz. To meet these specifications, an internal preamplifier must also be ordered with the noise figure option. In addition, these noise figure applications are code-compatible with older Keysight noise figure solutions for similar measurements.

## Features

- Fully specified to 26.5 GHz with optional internal preamplifier on the CXA or MXA signal analyzer
- Analyzers with frequency range options 526, 543, 544, or 550 can be used with block downconverters for noise figure measurements up to 110 GHz
- Works with Keysight N4000A smart noise sources and 346 Series noise sources
- Internal measurement uncertainty calculator

## Literature resources

- W/N9069C Noise Figure Measurement Application, Technical Overview with Self-Guided Demonstration, literature number 5992-0851EN

# Block Downconversion: Noise Figure Measurements Up to 110 GHz



Make noise figure measurements up to 110 GHz with either the NFA N8975B, N8976B or MXA N9020A-526 or the PXA N9030A-526.

Keysight K-Series block downconverters extend the upper frequency limit of the N8975B, N8976B, N9020A-526, or N9030A-526 from 26.5 GHz up to 110 GHz. The downconverter uses an internal LO to down convert the input signal to an IF that is within the measurement range. The K-Series is offered in 13.5 GHz bands. For example, a customer that would like to do noise figure measurements to 52 GHz would order K40, K50, and K63 in order to bridge from the 26.5 GHz end frequency of their instrument to 52 GHz.

## Block downconverter options

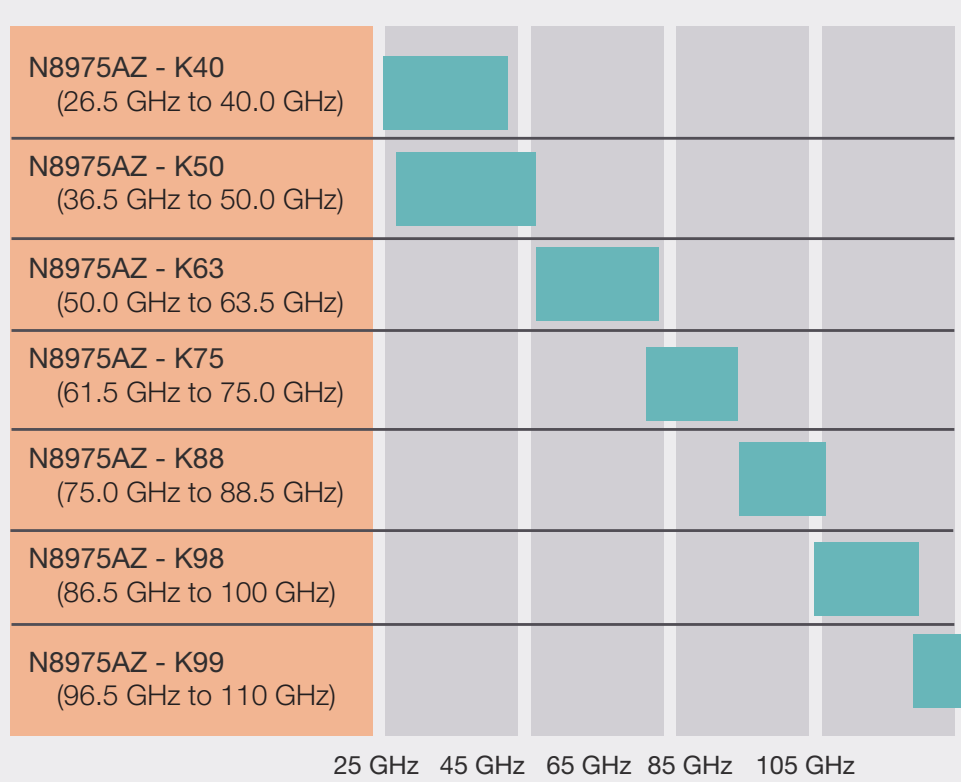



Figure 4. K-Series block downconverter frequency range chart.

# Noise Figure Measurements with the Highest Accuracy in the Industry



PNA-X microwave network analyzer

- N5241A
- N5242A
- N5244A
- N5245A

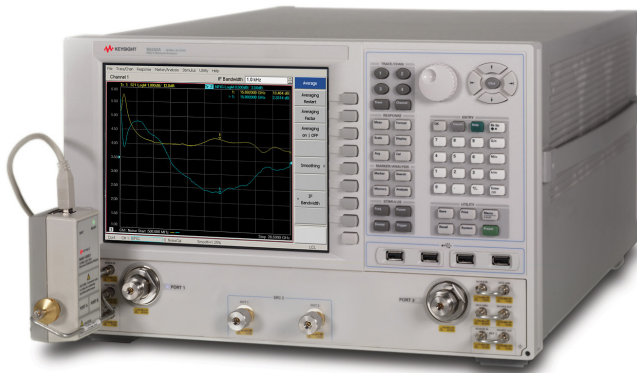

The Keysight PNA-X is the industry standard for high-performance microwave network analysis from 10 MHz to 50 GHz. This 2- or 4-port network analyzer offers a flexible, single-connection solution for S-parameter, noise figure, intermodulation distortion, compression, and pulsed-RF measurements. Keysight's unique source-corrected noise figure method (Options 028, 029, and H29) builds on the integrated, vector-error-corrected cold-source technique pioneered by the Keysight 8510 network analyzer. Using the PNA-X and an Keysight ECal module configured as an impedance tuner, mismatch and noise-parameter errors due to imperfect system source match are removed, greatly improving the accuracy of the cold-source technique. This approach surpasses the accuracy provided by today's Y-factor-based noise figure analyzers or spectrum analyzer solutions. With this option built directly into the Keysight PNA-X, the solution provides a complete single-connection, multiple-measurement package for R&D and manufacturing engineers developing and testing low-noise transistors, amplifiers, and transmit/receive (T/R) modules.

## Features

- Unique measurement technique provides the highest accuracy of any noise figure solution on the market
- Measure S-parameters, noise figure, compression, and intermodulation distortion with a single connection to the DUT
- Typically four to ten times faster than NFA (using 51 or 201 points)
- Works with coaxial, in-fixture, or on-wafer devices
- Hard specifications from 10 MHz to 50 GHz

## Literature resources

- PNA Series Brochure, literature number 5990-4592EN
- PNA Series Configuration Guide, literature number 5989-7606EN
- PNA-X Data Sheet, literature number N5242-90007
- High Accuracy Noise Figure Measurements Using the PNA-X Series Network Analyzer application note, literature number 5990-5800EN

## Automatically Downloads ENR Tables To Your Instrument



### SNS Series smart noise sources

- N4000A
- N4001A
- N4002A

The SNS Series noise sources can be used in conjunction with the X-Series signal analyzers, dedicated noise figure analyzers (NFA), and ESA spectrum analyzers. The SNS noise sources replicate the ENR output and frequency coverage of the traditional 346 Series noise sources; however, they have added benefits. The ENR data is stored in an EPROM and is automatically downloaded to the instrument, saving the need to manually enter the values into the calibration table at each cardinal frequency point. Another key benefit is that a thermistor is built into the noise source to continually update the analyzer with the correct temperature, yielding more accurate measurements due to automatic temperature compensation/correction.

### Features

- Electronic storage of ENR calibration data decreases the opportunity for user error
- Automatic download of ENR data to the instrument speeds overall set-up time
- Temperature compensation improves measurement accuracy leading to tighter specifications

### Literature resources

- SNS Technical Overview, literature number 5988-0081EN



## Keysight's Most Popular Noise Source Series



### 346 Series traditional noise sources

- 346A
- 346B
- 346C

The traditional and cost-effective noise source is the 346 Series, which operates with the full range of Keysight noise figure solutions. The 346 Series is categorized by its frequency coverage as well as ENR. Some active devices are sensitive to port match. They exhibit different noise figure values dependent on the source impedance. Noise sources will change their port impedance (SWR) as they are switched from T Hot to T Cold. Noise sources like the 346A have output circuitry that will minimize the impedance changes.

*Note: Keysight offers the 346CK01, 1 to 50 GHz and 346CK40, 1 to 40 GHz noise sources. The 346CK40 ships standard with the N8976B, NFA X-Series noise figure analyzer.*

### Features

- Low SWR for reducing noise figure measurement uncertainty
- Individually calibrated ENR values at specific frequencies
- Calibration supplied on floppy disk for easy loading into NFA Series noise figure analyzers

### Literature resources

- Keysight 346A/B/C Noise Sources: 10 MHz to 26.5 GHz, literature number 5953-6452B

## Noise Source Solution for Millimeter-Wave Devices



347 Series high frequency noise sources

- R347B
- Q347B



These waveguide noise sources allow you to make accurate and convenient noise figure measurements on millimeter-wave devices. The 347 Series provides extremely precise broadband noise at the input of the system or component under test. The noise figure meter then processes the ON/OFF ratio of noise power present in the system IF, and provides an accurate reading of noise figure and gain. These noise sources have remarkable ENR stability over time, which allows longer recalibration cycles and more accurate noise figure measurements.

### Features

- Performance and reliability at millimeter-wave frequencies
- Excellent ENR stability over time
- Low SWR

### Web resources

- [www.keysight.com/find/SNS](http://www.keysight.com/find/SNS) (select 347 Noise Source Family)

## Fast, Repeatable Calibrations with Confidence



### Noise source test set

- N2002A



The Keysight N2002A noise source test set is a stand-alone instrument that, as part of a calibration system, enables fast, repeatable calibrations with minimal levels of uncertainty. It is needed when making ENR tests on a noise source. This low-cost, easy-to-use test set ensures accurate calibration results, increasing measurement confidence and allowing the development of DUTs with tighter specifications. The N2002A noise source test set operates over a frequency range of 10.0 MHz to 26.5 GHz.

### Features

- Reduces noise figure uncertainty to ensure accurate and repeatable results
- Results traceable to national standards
- Full calibration of all Keysight SNS and 346 noise sources
- Manual control or remote operations using GPIB

### Literature resources

- N2002A Noise Source Test Set User's Guide, literature number N2002-90001
- Using the Keysight N8975A Noise Figure Analyzer and the N2002A Noise Source Test Set, literature number 5988-7229EN

## Additional Resources

### Literature

- 10 Hints for Making Successful Noise Figure Measurements (AN 57-3), literature number 5980-0288E
- Fundamentals of RF and Microwave Noise Figure Measurement (AN 57-1), literature number 5952-8255E
- Noise Figure Measurement Accuracy: The Y-Factor Method (AN 57-2), literature number 5952-3760E
- Noise Figure Measurements of Frequency Converting Devices (AN 1487), literature number 5989-0400EN
- Non-Zero Noise Figure After Calibration (AN 1484), literature number 5989-0270EN
- Practical Noise Figure Measurement and Analysis for Low-Noise Amplifier Designs (AN 1354), literature number 5980-1916E
- High-Accuracy Noise Figure Measurements Using the PNA-X Series Network Analyzer (AN 1408-20), literature number 5990-5800EN
- 5 Reasons to Buy the X-Series NFA, literature number 5992-1269EN

### Web

- Noise figure solutions: [www.keysight.com/find/noisefigure](http://www.keysight.com/find/noisefigure)
- Hints for Making Better Noise Figure Measurements - video series [www.keysight.com/find/noisefigurevideos](http://www.keysight.com/find/noisefigurevideos)

Learn more at: [www.keysight.com](http://www.keysight.com)

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: [www.keysight.com/find/contactus](http://www.keysight.com/find/contactus)

