

Keysight N9911X Economical Waveguide Calibration Components

NOTICE: This document contains references to Agilent Technologies. Agilent's former Test and Measurement business has become Keysight Technologies. For more information, go to **www.keysight.com**.



Notices

© Keysight Technologies 2013, 2014

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies as governed by United States and international copyright laws.

Manual Part Number

N9911-90002

Edition

August 2014

Keysight Technologies
1400 Fountaingrove Parkway
Santa Rosa, CA 95403

Warranty

The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Keysight disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Keysight shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Keysight and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as “Restricted computer software” as defined in FAR

52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Keysight Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

Printing Copies of Documentation from the Web

To print copies of documentation from the Web, download the PDF file from the Keysight web site:

- Go to <http://www.keysight.com>.
- Enter the product model number (Ex: N9911X) in the **Search** bar.
- Click **Search**.
- Click the **Manuals** hyperlink.
- Click the hyperlink title for the document you want to print - this downloads the PDF
- Print the document after the PDF has fully downloaded.

Contents

1. General Information	
Overview	1-2
Recording the Components Serial Numbers	1-3
Preventive Maintenance	1-7
When to Calibrate the Analyzer	1-7
How to Calibrate the Analyzer	1-7
2. Specifications	
Environmental Requirements	2-2
Temperature—What to Watch Out For	2-2
Typical VSWR Values	2-3
Instrument Interface Specifications	2-4
Dimension Specifications	2-5
3. Use, Maintenance, and Care of the Components	
Electrostatic Discharge	3-2
Visual Inspection	3-3
Cleaning the Mating Plane Surfaces	3-4
Connections	3-5
Aligning Two Precision Flanges	3-5
Tightening a Flange Connection	3-7
Inspecting a Flange Connection	3-7
Connecting a Termination to a Waveguide-to-Coax Adapter	3-8
Connecting an Offset Shim Between a Flush Short and Waveguide-to-Coax Adapter	3-8
Connecting a Flush Short to a Waveguide-to-Coax Adapter	3-9
Handling and Storage	3-10
4. Troubleshooting	
Troubleshooting Process	4-2
Where to Look for More Information	4-3
Returning a Component to Keysight	4-3
Contacting Keysight	4-4
5. Component Dimensions	
Flange Dimensions	5-5
Waveguide-to-Coax Adapter Dimensions	5-10
Termination Dimensions	5-18
Offset Shim Dimensions	5-26
Flush Short Dimensions	5-34

1 General Information

Overview

N9911X Economical Waveguide Calibration Components are used to calibrate FieldFox analyzers. With the calibration data properly loaded in the analyzer and a measurement calibration completed, systematic errors are minimized. For information on components available to purchase, refer to the online document *Keysight N9911X Economical Waveguide Calibration Components Configuration Guide* (part number N9911-90003).

Recording the Components Serial Numbers

The N9911X Economical Waveguide Components are individually serialized (serial numbers are labeled onto the body of each component). Record these serial numbers in the appropriate table. Recording the serial numbers will prevent confusion with similar components.

The N9911X calibration components are manufactured by Flann Microwave. Each component is imprinted with a Flann logo, part ID number, and serial number. To determine the Keysight option number for a component, use the cross-references in the following tables.

Table 1-1 Serial Number Record, Waveguide Designators C-Band/WR137/WG14, 5.38 – 8.18 GHz

Description	Component Serial Number	Keysight Option Number	Flann Part ID Number
Calibration Components – Metric			
Adapter 1, waveguide to type-N (male) coax		N9911X–110	14091–NM70–6332
Adapter 2, waveguide to type-N (male) coax		N9911X–110	14091–NM70–6332
Termination		N9911X–111	14045–6333
Flush short		N9911X–112	14191–6334
¼ wavelength offset shim		N9911X–113	14491–02–6335
Calibration Components – English (Imperial)			
Adapter 1, waveguide to type-N (male) coax		N9911X–115	14091–NM70–6136
Adapter 2, waveguide to type-N (male) coax		N9911X–115	14091–NM70–6136
Termination		N9911X–116	14045–3703
Flush short		N9911X–117	14191–704
¼ wavelength offset shim		N9911X–118	14491–02–3483

Recording the Components Serial Numbers**Table 1-2 Serial Number Record, Waveguide Designator X-Band/WR90/WG16, 8.2 – 12.5 GHz**

Description	Component Serial Number	Keysight Option Number	Flann Part ID Number
Calibration Components – Metric			
Adapter 1, waveguide to type-N (male) coax		N9911X–210	16091–NM70–6336
Adapter 2, waveguide to type-N (male) coax		N9911X–210	16091–NM70–6336
Termination		N9911X–211	16045–6337
Flush short		N9911X–212	16191–6338
$\frac{1}{4}$ wavelength offset shim		N9911X–213	16491–02–6339
Calibration Components – English (Imperial)			
Adapter 1, waveguide to type-N (male) coax		N9911X–215	16091–NM70–6141
Adapter 2, waveguide to type-N (male) coax		N9911X–215	16091–NM70–6141
Termination		N9911X–216	16045–5509
Flush short		N9911X–217	16191–2547
$\frac{1}{4}$ wavelength offset shim		N9911X–218	16491–02–2401

Table 1-3 Serial Number Record, Waveguide Designator Ku-Band/WR62/WG18, 11.9 – 18 GHz

Description	Component Serial Number	Keysight Option Number	Flann Part ID Number
Calibration Components – Metric			
Adapter 1, waveguide to type-N (male) coax		N9911X–310	18091–NM–6340
Adapter 2, waveguide to type-N (male) coax		N9911X–310	18091–NM–6340
Termination		N9911X–311	18045–6341
Flush short		N9911X–312	18191–6342
¼ wavelength offset shim		N9911X–313	18491–02–6343
Calibration Components – English (Imperial)			
Adapter 1, waveguide to type-N (male) coax		N9911X–315	18091–NM–6024
Adapter 2, waveguide to type-N (male) coax		N9911X–315	18091–NM–6024
Termination		N9911X–316	18045–2546
Flush short		N9911X–317	18191–4127
¼ wavelength offset shim		N9911X–318	18491–02–4095

Recording the Components Serial Numbers**Table 1-4 Serial Number Record, Waveguide Designator K-Band/WR42/WG20, 17.6 – 26.7 GHz**

Description	Component Serial Number	Keysight Option Number	Flann Part ID Number
Calibration Components – Metric			
Adapter 1, waveguide to 3.5 mm (male) coax		N9911X–310	20091–JM–2371
Adapter 2, waveguide to 3.5 mm (male) coax		N9911X–310	20091–JM–2371
Termination		N9911X–311	20045–2376
Flush short		N9911X–312	20191–6349
¼ wavelength offset shim		N9911X–313	20491–02–6351
Calibration Components – English (Imperial)			
Adapter 1, waveguide to 3.5 mm (male) coax		N9911X–315	20091–JM–2372
Adapter 2, waveguide to 3.5 mm (male) coax		N9911X–315	20091–JM–2372
Termination		N9911X–316	20045–5174
Flush short		N9911X–317	20191–6348
¼ wavelength offset shim		N9911X–318	20491–02–6350

Preventive Maintenance

The best techniques for maintaining the integrity of the components include:

- routine visual inspection
- routine cleaning
- proper connection techniques

All of these are described in [Chapter 3](#). Failure to detect and remove dirt or metallic particles on a mating plane surface can degrade repeatability and accuracy and can damage any component mated to it. Improper connections resulting from poor connection techniques, can also damage these components.

When to Calibrate the Analyzer

An analyzer calibration remains valid as long as the changes in the systematic error are insignificant. This means that changes to the uncorrected leakages (directivity and isolation), mismatches (source match and load match), and frequency response of the system are small (<10%) relative to accuracy specifications.

Change in the environment (especially temperature) between calibration and measurement is the major cause in calibration accuracy degradation. The major effect is a change in the physical length of external and internal cables. Other important causes are dirty and damaged test port connectors and calibration standards. If the connectors become dirty or damaged, measurement repeatability and accuracy is affected. Fortunately, it is relatively easy to evaluate the general validity of the calibration. To test repeatability, remeasure one of the calibration standards. If you can not obtain repeatable measurements from your calibration standards, maintenance needs to be performed on the test port connectors, cables and calibration standards. Also, maintain at least one sample of the device under test or some known device as your reference device.

How to Calibrate the Analyzer

Your analyzer's calibration user interface prompts you through each step in a 1-port or a 2-port calibration procedure. For detailed information on using your analyzer, refer to the appropriate user guide. See ["Where to Look for More Information"](#) on page 4-3.

2 Specifications

Environmental Requirements

Table 2-1 Environmental Requirements

Parameter	Limits
Temperature	
Operating ¹	+4 °C to +40 °C
Storage	-20 °C to +70 °C

1. The temperature range over which the calibration components maintain performance to their specifications.

Temperature—What to Watch Out For

Changes in temperature can affect electrical characteristics. Therefore, the operating temperature is a critical factor in performance. During a measurement calibration, the temperature of the calibration components must be stable and within the range shown in

Table 2-1.

IMPORTANT Avoid unnecessary handling of the components during calibration because your fingers act as a heat source and may increase the temperature of the component.

Typical VSWR Values

Table 2-2 and Table 2-3 list the typical VSWR values for the N9911X terminations and waveguide-to-coax adapters.

Table 2-2 Typical VSWR Values for Terminations

Keysight Option Number for Termination	Waveguide Band Designator	Thread Type	Frequency	VSWR, Maximum
N9911X-111	C-Band, WR137, WG14	Metric	5.38 to 8.18 GHz	1.10
N9911X-116		English (Imperial)		1.02
N9911X-211	X-Band, WR90, WG16	Metric	8.2 to 12.5 GHz	1.02
N9911X-216		English (Imperial)		
N9911X-311	Ku-Band, WR62, WG18	Metric	11.9 to 18 GHz	1.02
N9911X-316		English (Imperial)		
N9911X-411	K-Band, WR42, WG20	Metric	17.6 to 26.7GHz	1.03
N9911X-416		English (Imperial)		

Table 2-3 Typical VSWR Values for Waveguide-to-Coax Adapters

Keysight Option Number for Adapter	Waveguide Band Designator	Thread Type	Frequency	VSWR, Maximum
N9911X-110	C-Band, WR137, WG14	Metric	5.38 to 8.18 GHz	1.10
N9911X-115		English (Imperial)		
N9911X-210	X-Band, WR90, WG16	Metric	8.2 to 12.5 GHz	1.10
N9911X-215		English (Imperial)		
N9911X-310	Ku-Band, WR62, WG18	Metric	11.9 to 18 GHz	1.10
N9911X-315		English (Imperial)		
N9911X-410	K-Band, WR42, WG20	Metric	17.6 to 26.7GHz	1.20
N9911X-415		English (Imperial)		

Instrument Interface Specifications

Table 2-4 N9911X Instrument Interface Specifications

Waveguide Band Designator	Thread Type	Compatible Flange Type
C-Band/ WR137/ WG14	Metric	Flange (UAR 70, PAR 70, CAR 70, UDR 70, RDR 70, PDR 70)
	English (Imperial)	Flange (UG-441/U, UG-344/U, UG-343B/U, UG-440B/U, UG-1733/U, UG-1732/U, UG-1356/U, UG-1357/U, CPR 137F, CPR 137G)
X-Band/ WR90/ WG16	Metric	Flange (UBR 100, PBR 100, CBR 100, UDR 100, PDR 100, RDR 100)
	English (Imperial)	Flange (UG-39/U, UG-135/U, M3922/53-009, M3922/53-010, M3922/53-015, M3922/53-016, UG-40B/U, UG-136B/U, M3922/59-013, M3922/59-014, UG-1736/U, UG-1737/U, UG-1360/U, UG-1361/U, CPR 90F, CPR 90G)
Ku-Band/ WR62/ WG18	Metric	Flange (UBR 140, PBR 140, CBR 140, UDR 140, PDR 140, RDR 140)
	English (Imperial)	Flange (UG-419A/U, UG-1665/U, M3922/53-011, M3922/53-012, M3922/53-017, M3922/53-018, UG-541A/U, UG-1666/U)
K-Band/ WR42/ WG20	Metric	Flange (UBR 220, PBR 220, CBR 220, UDR 220, PDR 220, RDR 220)
	English (Imperial)	Flange (UG-595/U, UG-597/U, UG596A/U, UG-598A/U, M3922/70-027, M3922/70-028)

Dimension Specifications

Table 2-5 N9911X Dimension Specifications

Component	Parameter	WR137	WR90	WR62	WR42
Adapter, waveguide-to-coax	Waveguide aperture tolerance	46 um MAX	25 um MAX	23 um MAX	20 um MAX
Termination	Waveguide aperture tolerance	46 um MAX	25 um MAX	23 um MAX	20 um MAX
Flush short	Shorting face flatness	25 um	25 um	25 um	25 um
1/4 wavelength offset shim	Waveguide aperture tolerance	46 um MAX, 14.711 mm +/- 45 um	25 um MAX, 9.63 mm +/- 35 um	23 um MAX, 6.668 mm +/- 30 um	20 um MAX, 4.501 mm +/- 25 um

NOTE Refer to the Appendix for graphics showing the component dimensions.

3 Use, Maintenance, and Care of the Components

Electrostatic Discharge


Protection against electrostatic discharge (ESD) is essential while connecting, inspecting, or cleaning connectors attached to a static-sensitive circuit (such as those found in test sets).

Static electricity can build up on your body and can easily damage sensitive internal circuit elements when discharged. Static discharges too small to be felt can cause permanent damage. Devices such as calibration components and devices under test (DUT), can also carry an electrostatic charge. To prevent damage to the test set, components, and devices:

- *always* wear a grounded wrist strap having a 1 MW resistor in series with it when handling components and devices or when making connections to the test set.
- *always* use a grounded antistatic mat in front of your test equipment.
- *always* wear a heel strap when working in an area with a conductive floor. If you are uncertain about the conductivity of your floor, wear a heel strap.
- *always* ground yourself before you clean, inspect, or make a connection to a static-sensitive device or test port. You can, for example, grasp the grounded outer shell of the test port or cable connector briefly.
- *always* ground the center conductor of a test cable before making a connection to the analyzer test port or other static-sensitive device. This can be done as follows:
 1. Connect a short to one end of the cable to short the center conductor to the outer conductor.
 2. While wearing a grounded wrist strap, grasp the outer shell of the cable connector.
 3. Connect the other end of the cable to the test port.
- Remove the short from the cable.

Figure 3-1 shows a typical ESD protection setup using a grounded mat and wrist strap.

Figure 3-1 ESD Protection Setup

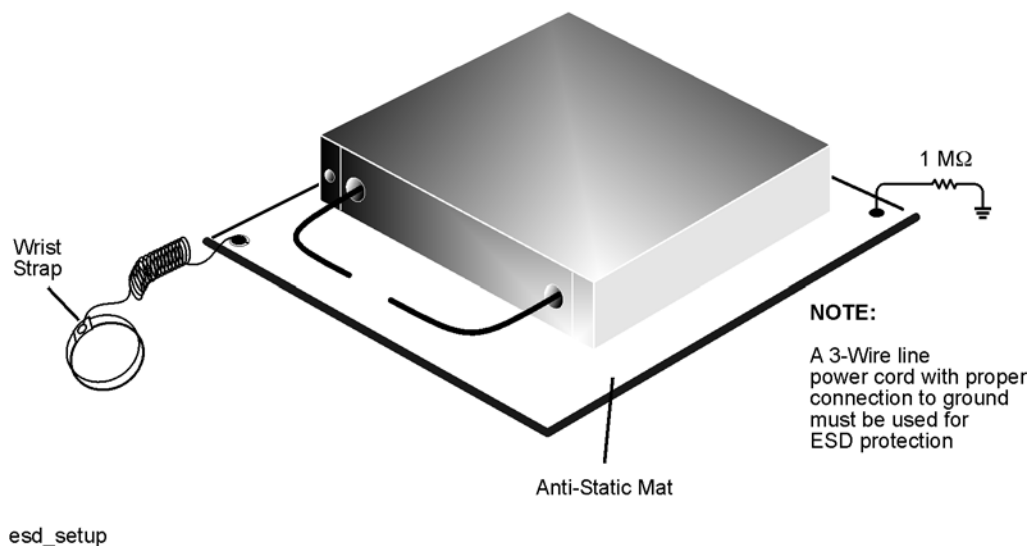

Visual Inspection

Visual inspection and, if necessary, cleaning should be done every time a connection is made. Inspect mating surfaces for dirt, dust, foreign particles, or scratches, which can degrade component performance. A damaged mating surface can damage any good surface connected to it. If necessary, clean all mating surfaces.

Magnification is helpful when inspecting mating surfaces, but it is not required and may actually be misleading. Defects and damage that cannot be seen without magnification generally have no effect on electrical or mechanical performance. Magnification is of great use in analyzing the nature and cause of damage and in cleaning mating surfaces, but it is not required for inspection.

Cleaning the Mating Plane Surfaces

1. Use Compressed Air or Nitrogen

WARNING Always use protective eyewear when using compressed air or nitrogen.

Use compressed air (or nitrogen) to loosen particles on the mating plane surfaces. Clean air cannot damage a component or leave particles or residues behind.

You can use any source of clean, dry, low-pressure compressed air or nitrogen that has an effective oil-vapor filter and liquid condensation trap placed just before the outlet hose.

Ground the hose nozzle to prevent electrostatic discharge, and set the air pressure to less than 414 kPa (60 psi) to control the velocity of the air stream. High-velocity streams of compressed air can cause electrostatic effects when directed into a component. These electrostatic effects can damage the component. Refer to “**Electrostatic Discharge**” earlier in this chapter for additional information.

WARNING Keep isopropyl alcohol away from heat, sparks, and flame. Store in a tightly closed container. It is extremely flammable. In case of fire, use alcohol foam, dry chemical, or carbon dioxide; water may be ineffective.

Use isopropyl alcohol with adequate ventilation and avoid contact with eyes, skin, and clothing. It causes skin irritation, may cause eye damage, and is harmful if swallowed or inhaled. It may be harmful if absorbed through the skin. Wash thoroughly after handling.

In case of spill, soak up with sand or earth. Flush spill area with water.

Dispose of isopropyl alcohol in accordance with all applicable federal, state, and local environmental regulations.

2. Clean the Mating Plane Surfaces

- a. Apply a small amount of isopropyl alcohol to a lint-free cleaning swab.
- b. Clean the mating plane surfaces.
- c. Let the alcohol evaporate, then blow the mating plane surface dry with a gentle stream of clean, low-pressure compressed air or nitrogen. Always completely dry a component before you reassemble or use it.

3. Inspect

- a. Inspect the mating plane surface to make sure that no particles or residue remain. “**Visual Inspection**” on page 3-3.

Connections

Good connections require a skilled operator. Slight errors in operator technique can have a significant effect on measurements and measurement uncertainties. *The most common cause of measurement error is poor connections.*


The following procedures illustrate how to make good connections.

IMPORTANT Unlike threaded components, the WR-90, WR-62, WR-42 waveguide mating planes are flanges that you must carefully screw together. Always connect waveguide in the same flange orientation. For example, use the label as a reference and always connect components with the labels facing the same direction.

Aligning Two Precision Flanges

A precision flange has two precision alignment holes, as shown in [Figure 3-2](#). A non-precision flange has only screw holes.


Figure 3-2 Precision Alignment Holes

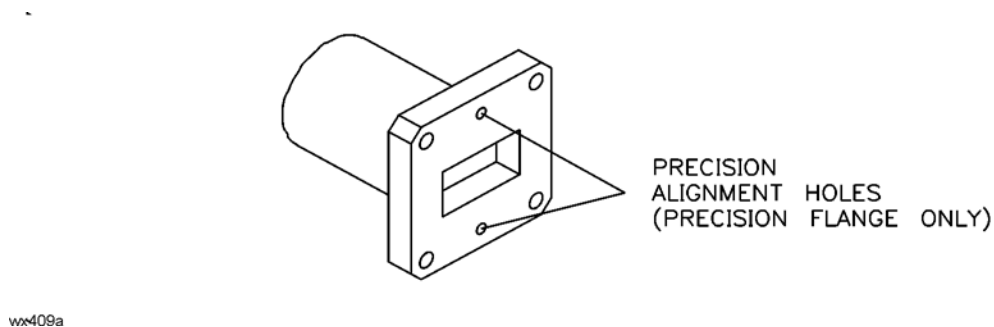

Connections


1. Place the slip pins in the top and bottom holes of one flange, as shown in [Figure 3-3](#).

Figure 3-3 Inserting Slip Pins

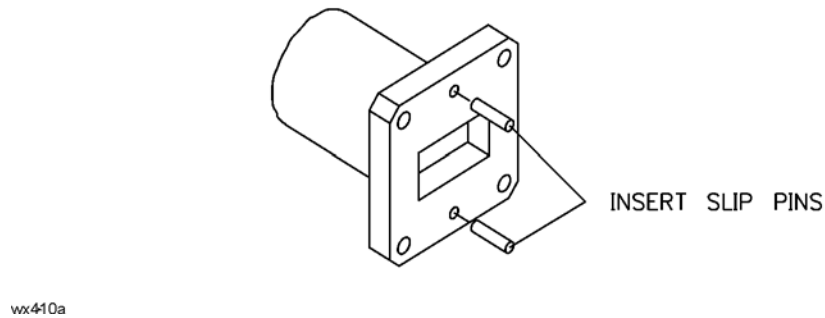

2. Using the pins as guides for the adapter, offset shim, and waveguide-to-coax adapter, carefully align the flanges and insert two screws in the diagonal corner holes, as shown in [Figure 3-4](#).

Figure 3-4 Aligning Flanges

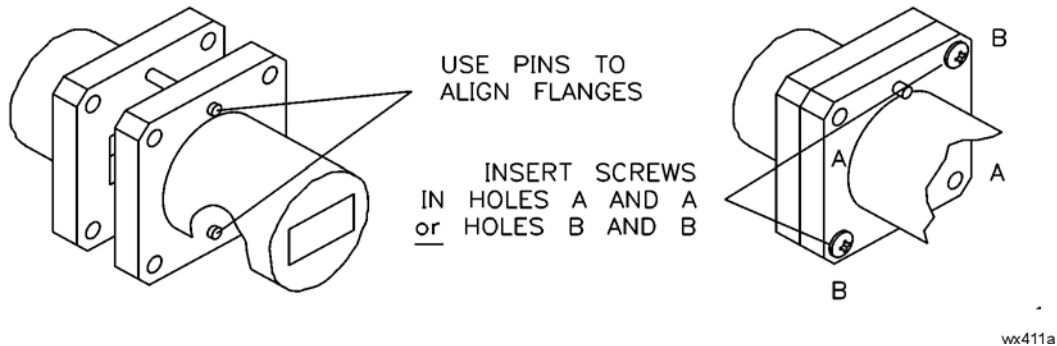


3. Place a lock washer and nut on each screw, and finger tighten.
4. Insert the remaining two screws.
5. Place a lock washer and nut on each screw, and finger tighten.
6. Remove the slip pins.
7. Go to ["Tightening a Flange Connection" on page 3-7](#).

Tightening a Flange Connection

NOTE The best connection has symmetrical pressure applied as you gradually tighten the screws.

1. In an "X" pattern (for equal compression), tighten all four screws using a hex ball driver. Do *not* over-tighten. See **Figure 3-5**.
2. Visually inspect the connection. Refer to the following section "**Inspecting a Flange Connection**."

Figure 3-5 "X" Screw Pattern

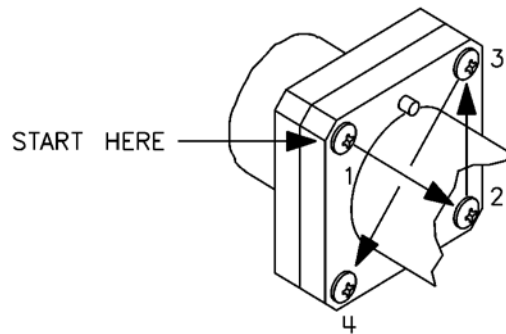

wx413a

Inspecting a Flange Connection


Inspect the flange connection as follows:

1. Place an electric light or white paper behind the connection.
2. Check the flange matings for any gap. A good connection has no gaps between the connected waveguide flanges, and the waveguide walls are flush. There is no step or offset.
3. Ensure that all four screws are equally tight.

Connections

Connecting a Termination to a Waveguide-to-Coax Adapter

Figure 3-6 Termination and Adapter

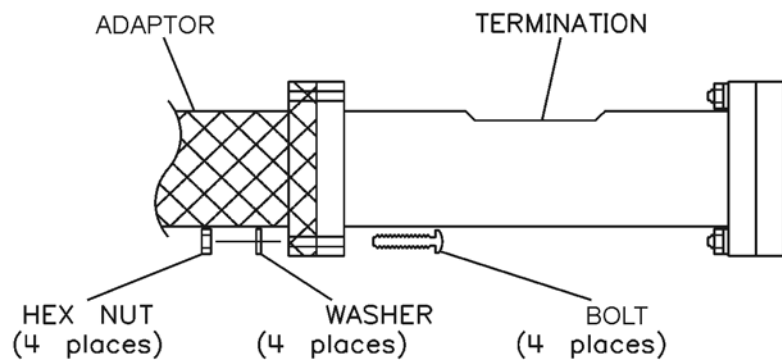


wx403a

Connecting an Offset Shim Between a Flush Short and Waveguide-to-Coax Adapter

Create an offset short by connecting the offset shim between the short and the appropriate adapter, as shown in [Figure 3-7](#).


Figure 3-7 Shim, Flush Short, and Adapter (Creates an Offset Short)

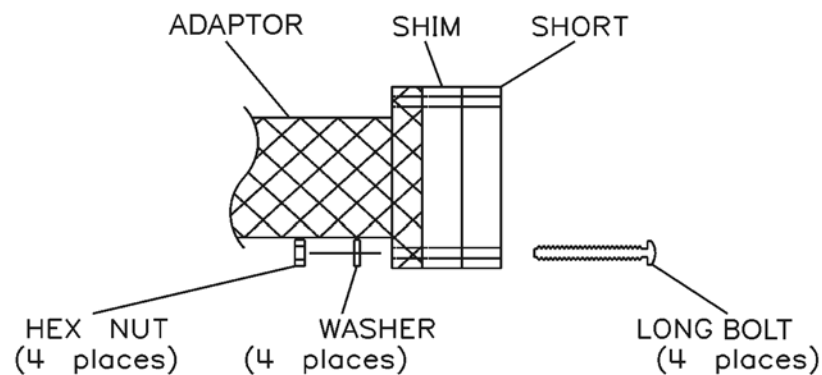

wx405a

Connecting a Flush Short to a Waveguide-to-Coax Adapter

Figure 3-8 Flush Short and Adapter

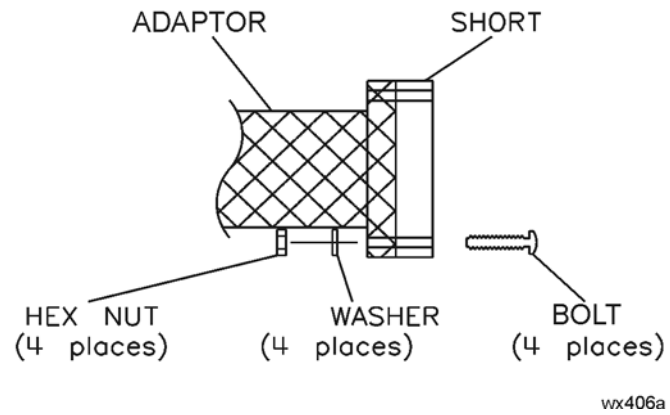

Handling and Storage


- Install the protective end caps and store the calibration components when not in use.
- Never store components loose in a box, or in a desk or bench drawer. This is the most common cause of component damage during storage.
- Keep components clean.
- Do not touch mating plane surfaces. Natural skin oils and microscopic particles of dirt are easily transferred to a component and are very difficult to remove.
- Do not set components contact-end down on a hard surface. The plating and the mating plane surfaces can be damaged if the interface comes in contact with any hard surface.

4 Troubleshooting

Troubleshooting Process

If you suspect a bad calibration, or if your analyzer does not pass performance verification, follow the steps in [Figure 4-1](#)

Figure 4-1 Troubleshooting Flowchart

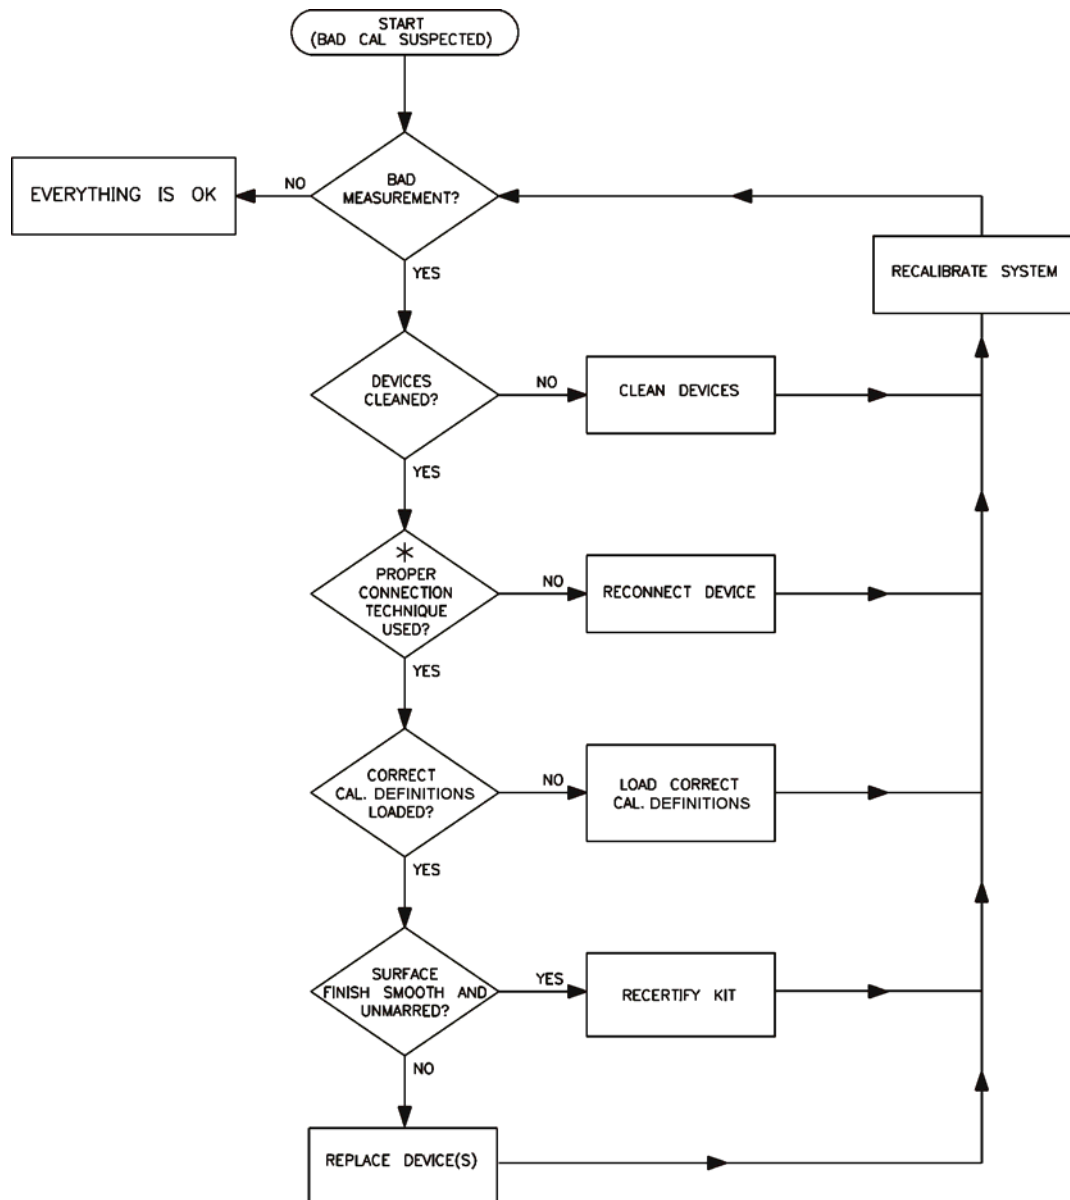

* NO GAPS; WAVEGUIDE WALLS FLUSH;
EVEN AND SYMMETRICAL TIGHTENING.

wx416a

Where to Look for More Information

This manual contains limited information about analyzer system operation. For detailed information on using a FieldFox analyzer, refer to the appropriate user guide.

To view an online FieldFox user guide, use the following steps:

1. Go to *www.keysight.com*.
2. Enter your FieldFox model number (Ex: N9928A) in the Search box and click **Search**.
3. Click **Manuals**.
4. Click the title/hyperlink for the document PDF you want to view.

If you need additional information, see [“Contacting Keysight” on page 4-4](#).

Returning a Component to Keysight

If an N9911X component requires service, contact Keysight Technologies for information on where to send it - see [“Contacting Keysight” on page 4-4](#). Please provide the following information:

- your company name and address
- a technical contact person within your company, and the person's complete telephone number
- the Keysight option number, Flann part ID number, and serial number of the component (refer to [“Recording the Components Serial Numbers” on page 1-3](#))
- the type of service required
- a *detailed* description of the problem and how the component was being used when the problem occurred

NOTE	When returning a component to Keysight, install the protective end caps on the component.
-------------	---

Contacting Keysight

Assistance with test and measurement needs and information on finding a local Keysight office are available on the Web at:

www.keysight.com/find/assist

If you do not have access to the Internet, please contact your Keysight field engineer.

NOTE	In any correspondence or telephone conversation, refer to the Keysight product by its model number and full serial number. With this information, the Keysight representative can determine whether your product is still within its warranty period.
-------------	---

5 Component Dimensions

Table 5-1 List of Figures

Figure Title and Location
"Flange, Waveguide Designators C-Band/WR137/WG14, Metric" on page 5-5
"Flange, Waveguide Designators C-Band/WR137/WG14, English (Imperial)" on page 5-6
"Flange, Waveguide Designators X-Band/WR90/WG16, Metric" on page 5-6
"Flange, Waveguide Designators X-Band/WR90/WG16, English (Imperial)" on page 5-7
"Flange, Waveguide Designators Ku-Band/WR62/WG18, Metric" on page 5-7
"Flange, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial)" on page 5-8
"Flange, Waveguide Designators K-Band/WR42/WG20, Metric" on page 5-8
"Flange, Waveguide Designators K-Band/WR42/WG20, English (Imperial)" on page 5-9
"Adapter, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-110" on page 5-10
"Adapter, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-115" on page 5-11
"Adapter, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-210" on page 5-12
"Adapter, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-215" on page 5-13
"Adapter, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-310" on page 5-14
"Adapter, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-315" on page 5-15
"Adapter, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-410" on page 5-16
"Adapter, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-415" on page 5-17
"Termination, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-111" on page 5-18

Table 5-1 List of Figures

Figure Title and Location
“Termination, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-116” on page 5-19
“Termination, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-211” on page 5-20
“Termination, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-216” on page 5-21
“Termination, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-311” on page 5-22
“Termination, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-316” on page 5-23
“Termination, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-411” on page 5-24
“Termination, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-416” on page 5-25
“Offset Shim, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-113” on page 5-26
“Offset Shim, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-118” on page 5-27
“Offset Shim, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-213” on page 5-28
“Offset Shim, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-218” on page 5-29
“Offset Shim, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-313” on page 5-30
“Offset Shim, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-318” on page 5-31
“Offset Shim, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-413” on page 5-32
“Offset Shim, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-418” on page 5-33
“Flush Short, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-112” on page 5-34

Table 5-1 List of Figures

Figure Title and Location
“Flush Short, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-117” on page 5-35
“Flush Short, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-212” on page 5-36
“Flush Short, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-217” on page 5-37
“Flush Short, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-312” on page 5-38
“Flush Short, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-317” on page 5-39
“Flush Short, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-412” on page 5-40
“Flush Short, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-417” on page 5-41

Flange Dimensions


NOTE The dimensions shown in the following graphics are in millimeters.

Figure 5-1 Flange, Waveguide Designators C-Band/WR137/WG14, Metric

UAR 70 HOLES	
HOLE	DESCRIPTION
A	Ø5.155±0.015 THRU
B	Ø5.38±0.24 THRU

UDR 70 HOLES	
HOLE	DESCRIPTION
C	$\phi 5.155 \pm 0.015$ THRU
D	$\phi 5.38 \pm 0.24$ THRU

DOWEL HOLES	
HOLE	DESCRIPTION
W	Ø ^{3.2} _{3.19} THRU ON FINISHED COMPONENTS

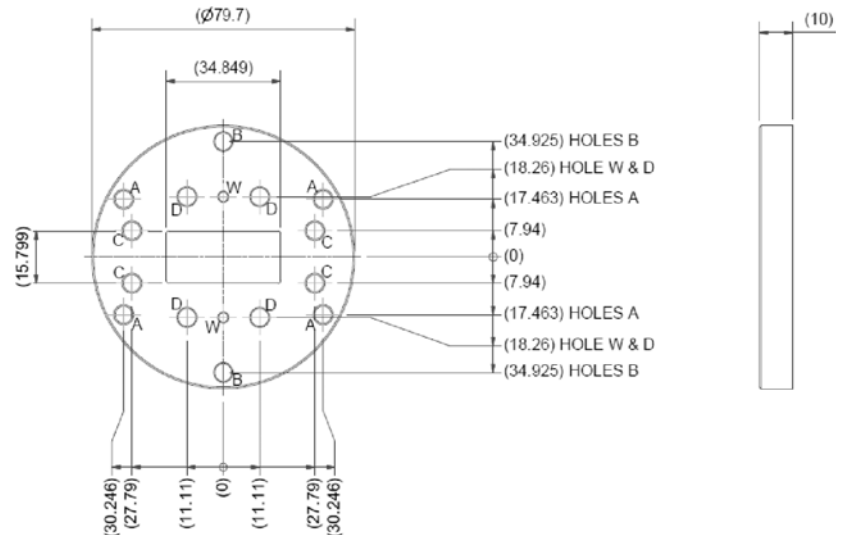

FLANGE PROFILE BASED ON:- UAR 70
FLANGE THICKNESS BASED ON:- UDR 70

INTERFACE COMPATIBLE WITH:-
UAR 70, PAR 70, CAR 70,
UDR 70, RDR 70, PDR 70

N9911_002_201

Flange Dimensions

Figure 5-2 Flange, Waveguide Designators C-Band/WR137/WG14, English (Imperial)


UG-344/U HOLES	
HOLE	DESCRIPTION
A	Ø5.105± 0.05 THRU

UG-1732/U HOLES	
HOLE	DESCRIPTION
C	Ø5.029±0.05 THRU

DOWEL HOLES	
HOLE	DESCRIPTION
W	$\varnothing \frac{3.2}{3.19}$ THRU ON FINISHED COMPONENTS

FLANGE PROFILE BASED ON:- UG-344/U
FLANGE THICKNESS BASED ON:- UDR 70

INTERFACE COMPATABLE WITH:-
UG-344/U, UG-441/U,
UG-343B/U, UG-440B/U
UG-1732/U, UG-1733/U, UG-1356/U, UG-1357/U,
CPR 137 F, CPR 137 G

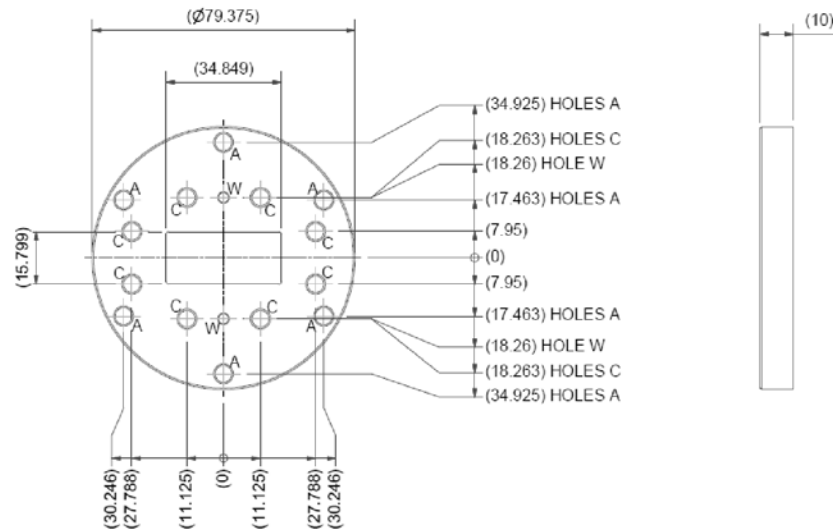

N9911_002_202

Figure 5-3 Flange, Waveguide Designators X-Band/WR90/WG16, Metric


UDR 100 HOLES	
HOLE	DESCRIPTION
A	Ø4.085± 0.015 THRU
B	Ø4.31± 0.24 THRU

UBR 100 HOLES	
HOLE	DESCRIPTION
C	Ø4.255±0.015 THRU

DOWEL HOLES	
HOLE	DESCRIPTION
W	Ø 3.2 3.19 THRU ON FINISHED COMPONENTS


FLANGE PROFILE BASED ON:- UDR 100
FLANGE THICKNESS BASED ON:- UDR 100

INTERFACE COMPATABLE WITH:-
UDR 100, RDR 100, PDR 100,
UBR 100, PBR 100, CBR 100

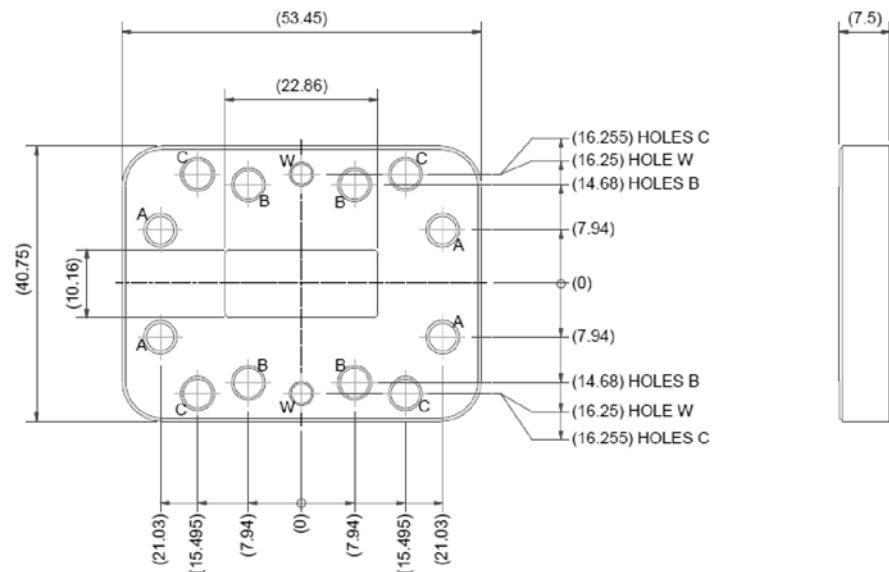


N9911_002_203

Figure 5-4 Flange, Waveguide Designators X-Band/WR90/WG16, English (Imperial)

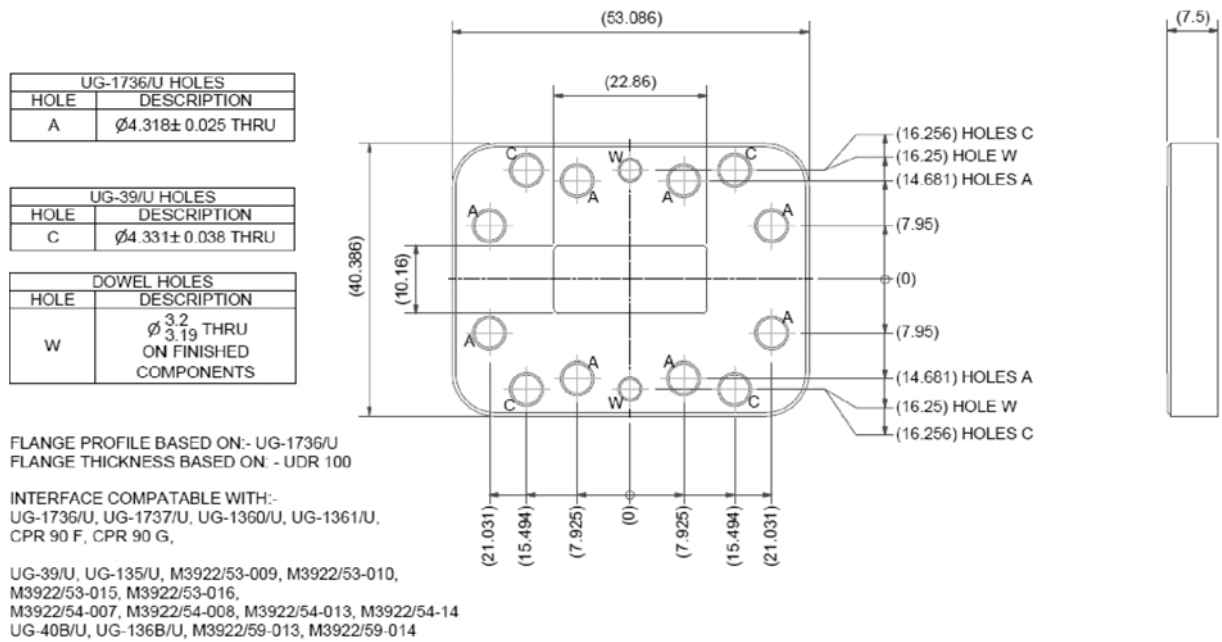

N9911_002_204


Figure 5-5 Flange, Waveguide Designators Ku-Band/WR62/WG18, Metric

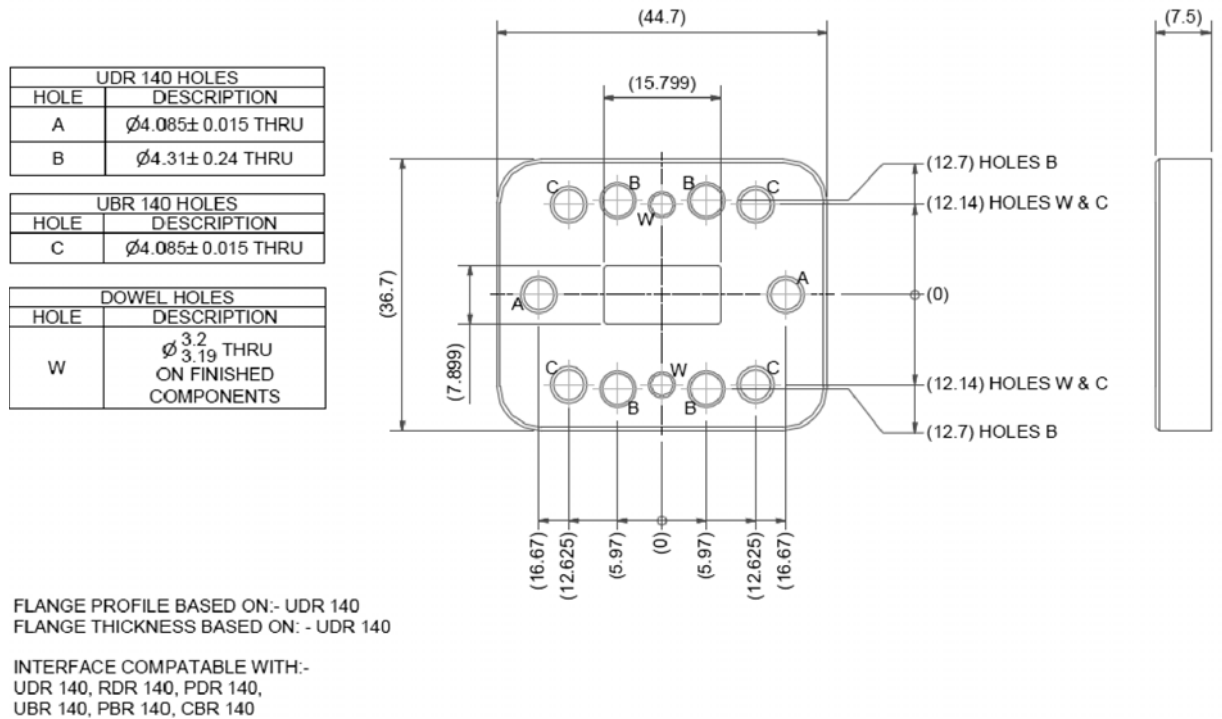

N9911_002_205

Flange Dimensions

Figure 5-6 Flange, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial)

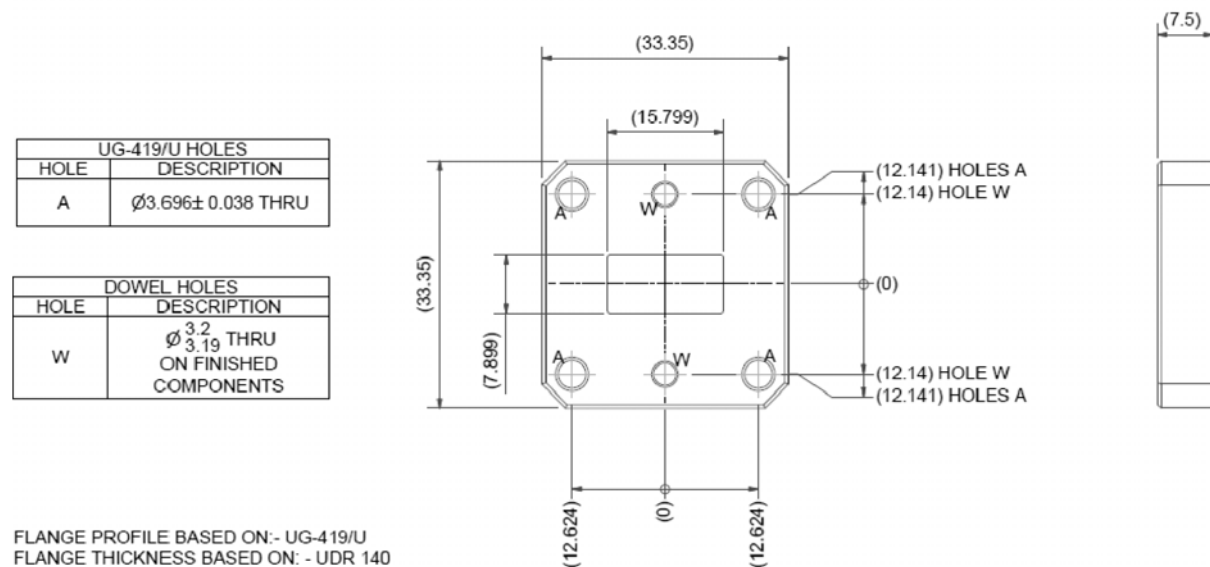


FLANGE PROFILE BASED ON:- UG-419/U
FLANGE THICKNESS BASED ON:- UDR 140

INTERFACE COMPATABLE WITH:-
UG-419/U, UG-1665/U,
M3922/53-011, M3922/53-012, M3922/53-017, M3922/53-018,
M3922/54-009, M3922/54-010,
UG-5414/U, UG-1666/U,
M3922/70-007, M3922/70-008, M3922/70-019, M3922/70-020,

N9911_002_206

Figure 5-7 Flange, Waveguide Designators K-Band/WR42/WG20, Metric

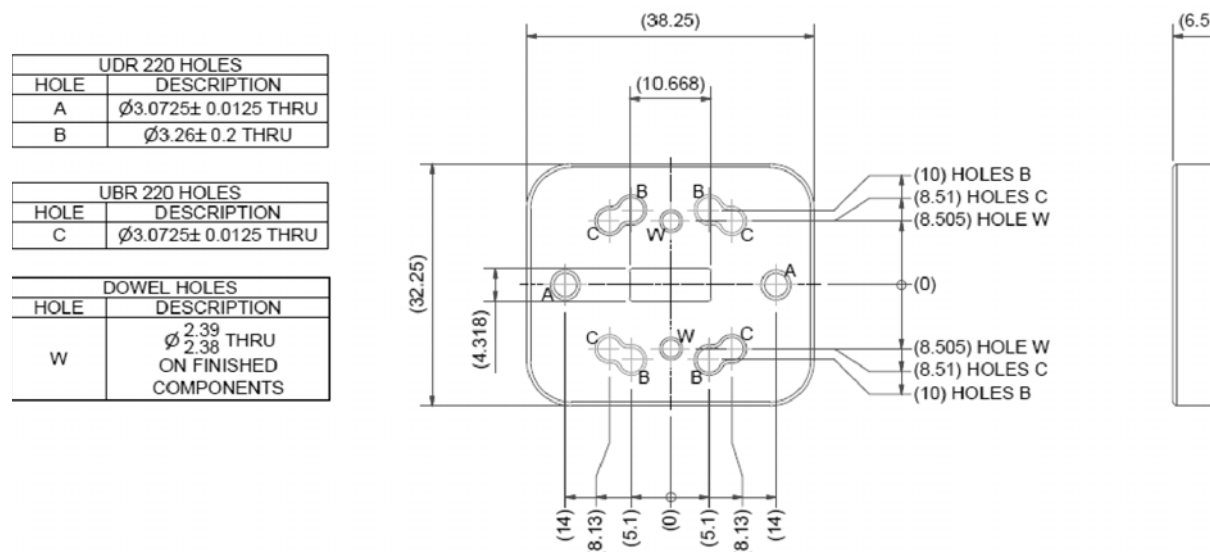


FLANGE PROFILE BASED ON:- UDR 220
FLANGE THICKNESS BASED ON:- UDR 220

INTERFACE COMPATIBLE WITH:-
UDR 220, RDR 220, PDR 220,
UBR 220, PBR 220, CBR 220

N9911 002 207

Figure 5-8 Flange, Waveguide Designators K-Band/WR42/WG20, English (Imperial)

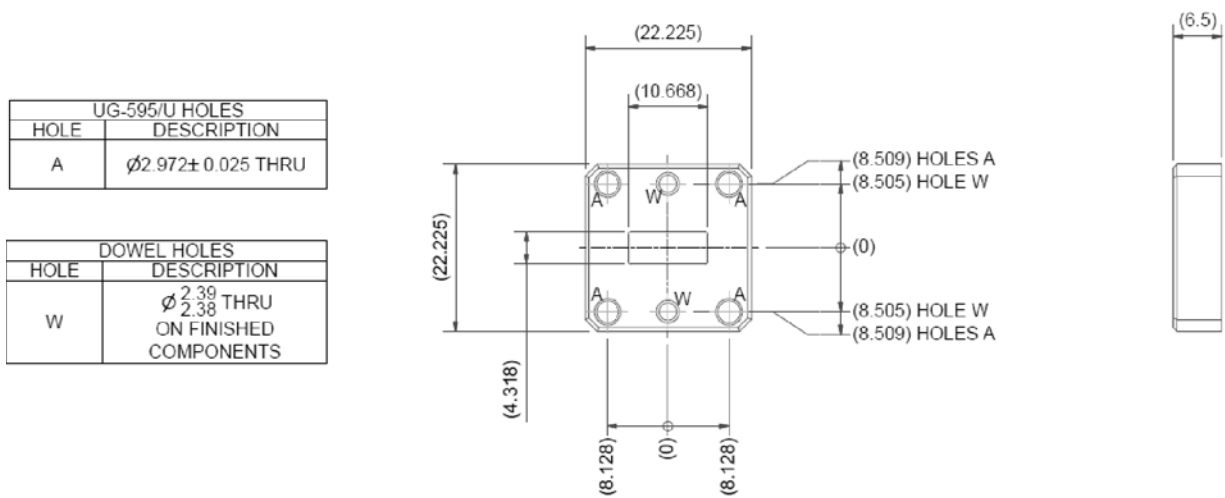

FLANGE PROFILE BASED ON:- UG-595/U
FLANGE THICKNESS BASED ON:- UDR 220


INTERFACE COMPATIBLE WITH:-
UG-595/U, UG-597/U,
UG-596A/U, UG598A/U,
M3922/70-027, M3922/70-028

N9911_002_208

Waveguide-to-Coax Adapter Dimensions


NOTE The dimensions shown in the following graphics are in millimeters.

Figure 5-9 Adapter, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-110

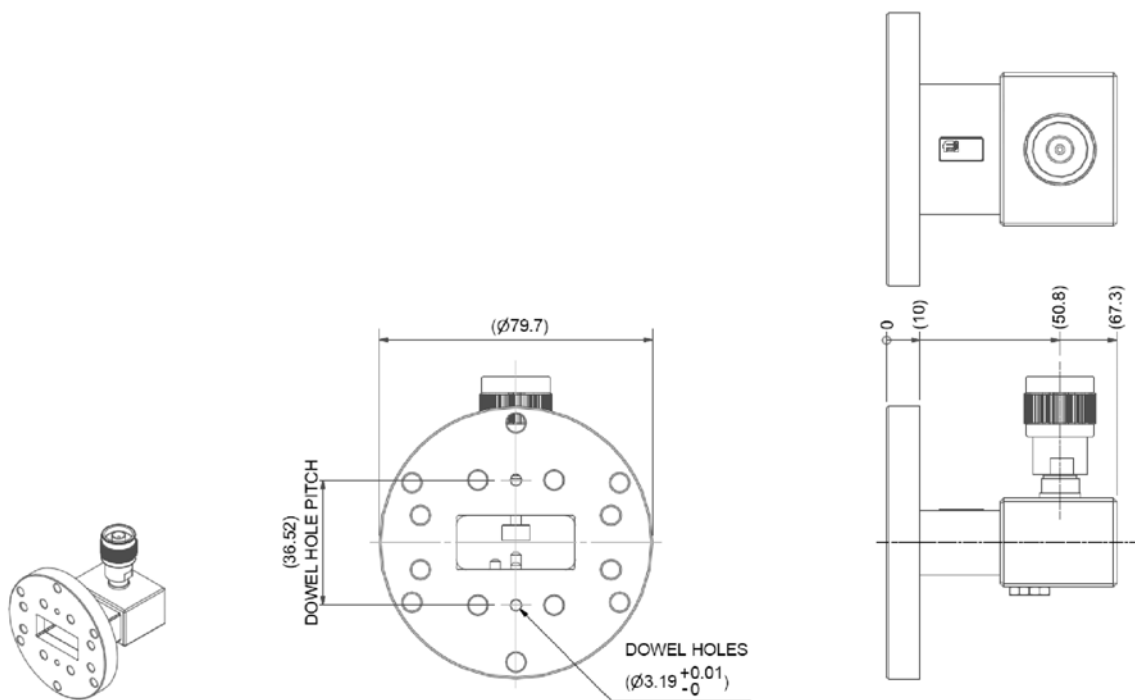

N9911_002_235


Figure 5-10 Adapter, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-115

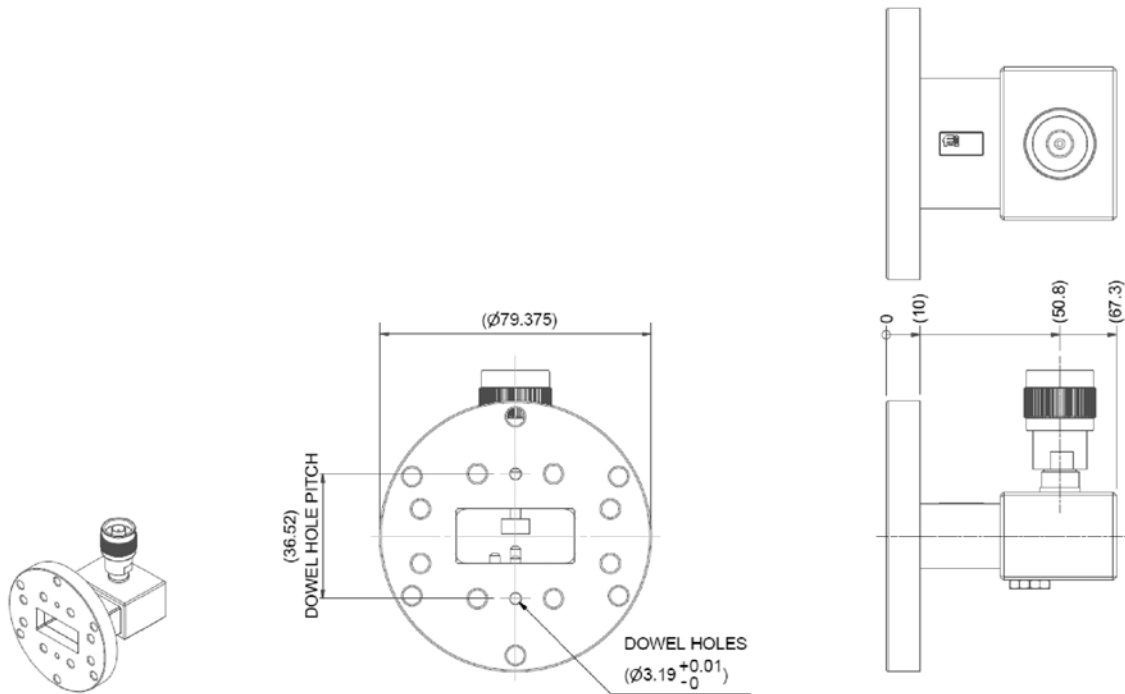

N9911_002_234


Waveguide-to-Coax Adapter Dimensions

Figure 5-11 Adapter, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-210

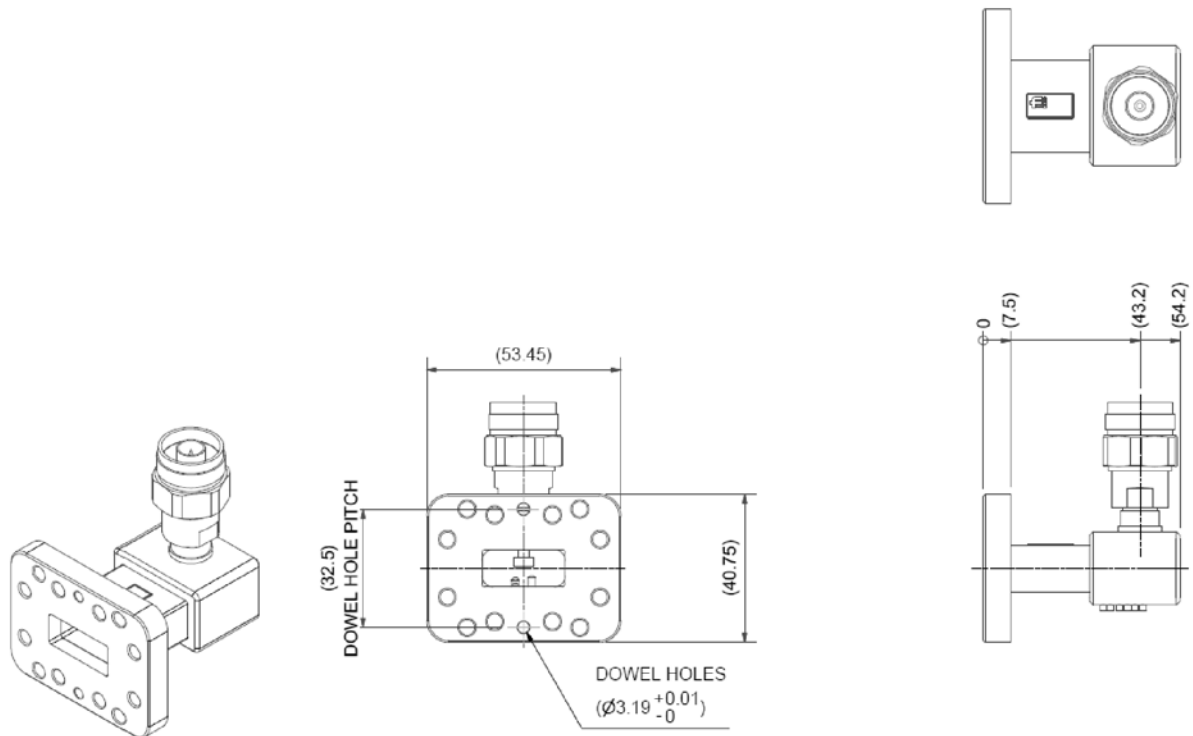

N9911_002_214

Figure 5-12 Adapter, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-215

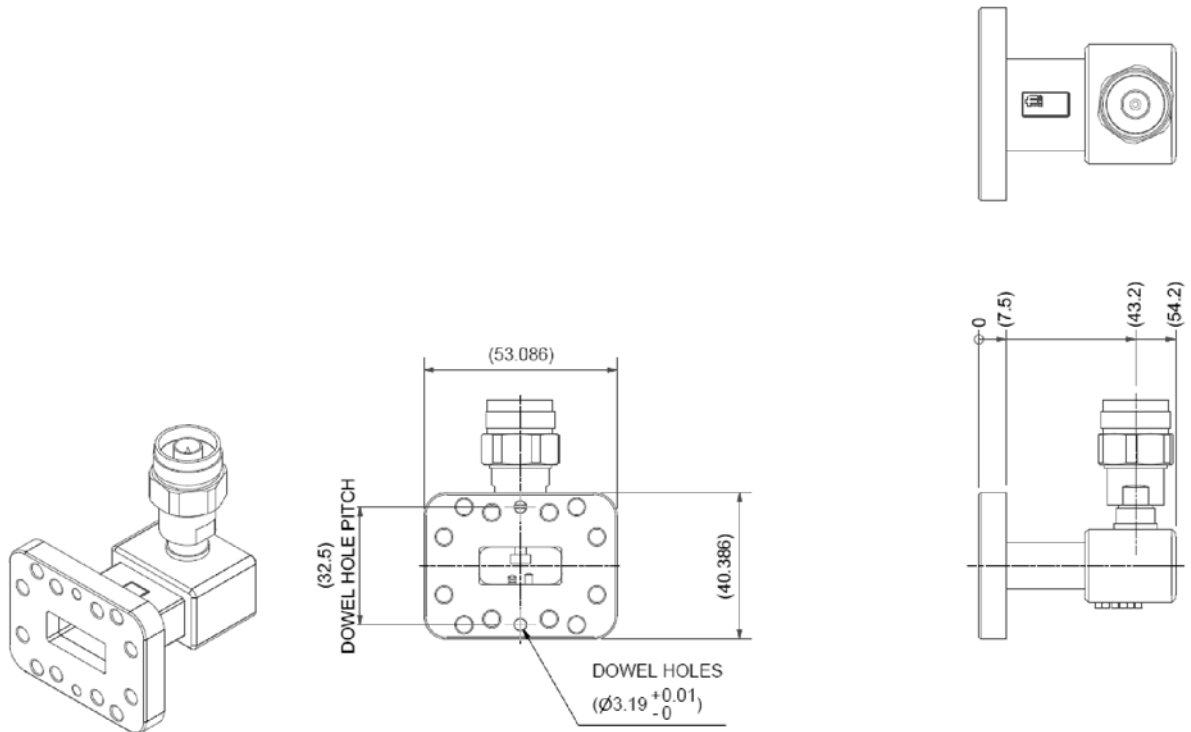


N9911_002_213

Technical drawing of the 100mm x 100mm x 10mm plate with a 10mm x 10mm hole and a 10mm x 10mm hole. The drawing includes three views: a perspective view, a top view, and a side view. The top view shows a 100mm x 100mm plate with a 10mm x 10mm hole in the center. The side view shows the plate thickness of 10mm. The drawing is labeled with dimensions in millimeters and inches.

User's Guide N9911-90002

Figure 5-14 Adapter, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight
Part Number N9911X-315

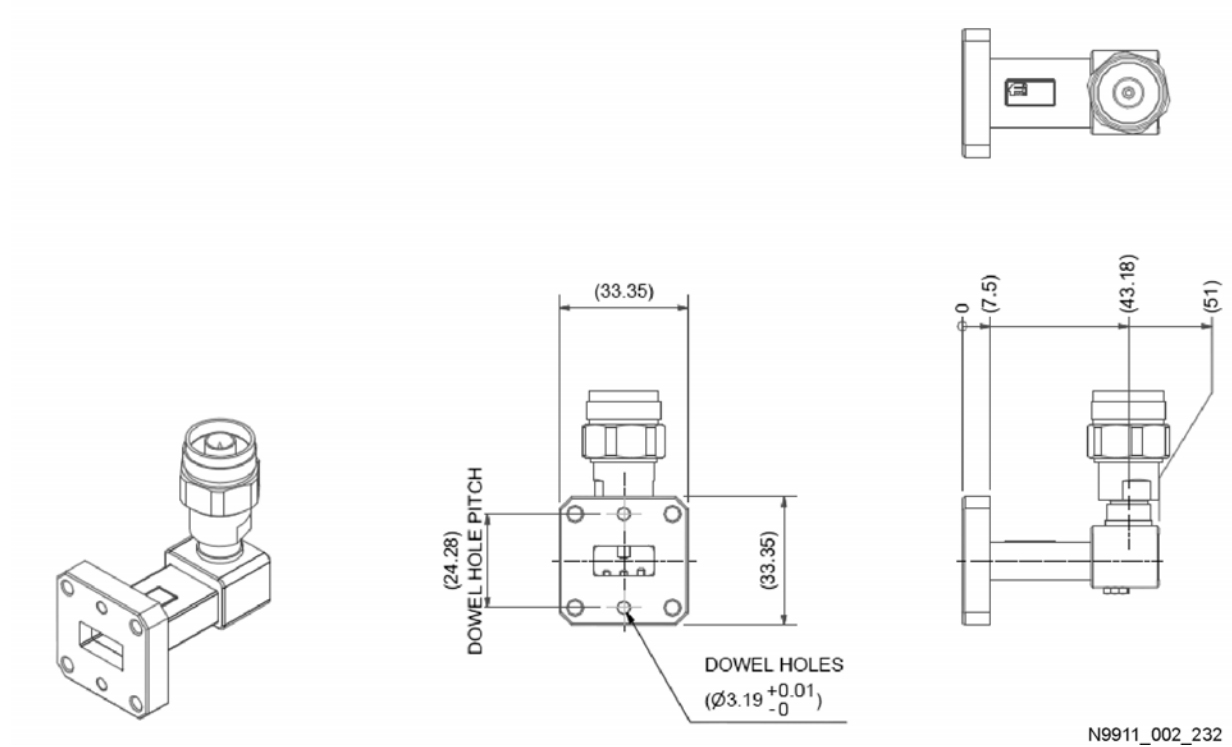

Technical drawing of the 100mm x 100mm x 10mm plate, showing dimensions and assembly details.

Dimensions:


- Overall width: 100 (38.25)
- Overall height: 100 (32.25)
- Dowel hole pitch: 17.01
- Dowel hole diameter: $\varnothing 2.38^{+0.01}_{-0}$

Assembly Details:

- The plate is shown with a 10mm thick base plate and a 10mm thick top plate.
- The plate is secured by a bolt and nut assembly.
- The plate is shown with a 10mm thick base plate and a 10mm thick top plate.

N9911_002_212

Figure 5-16 Adapter, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-415

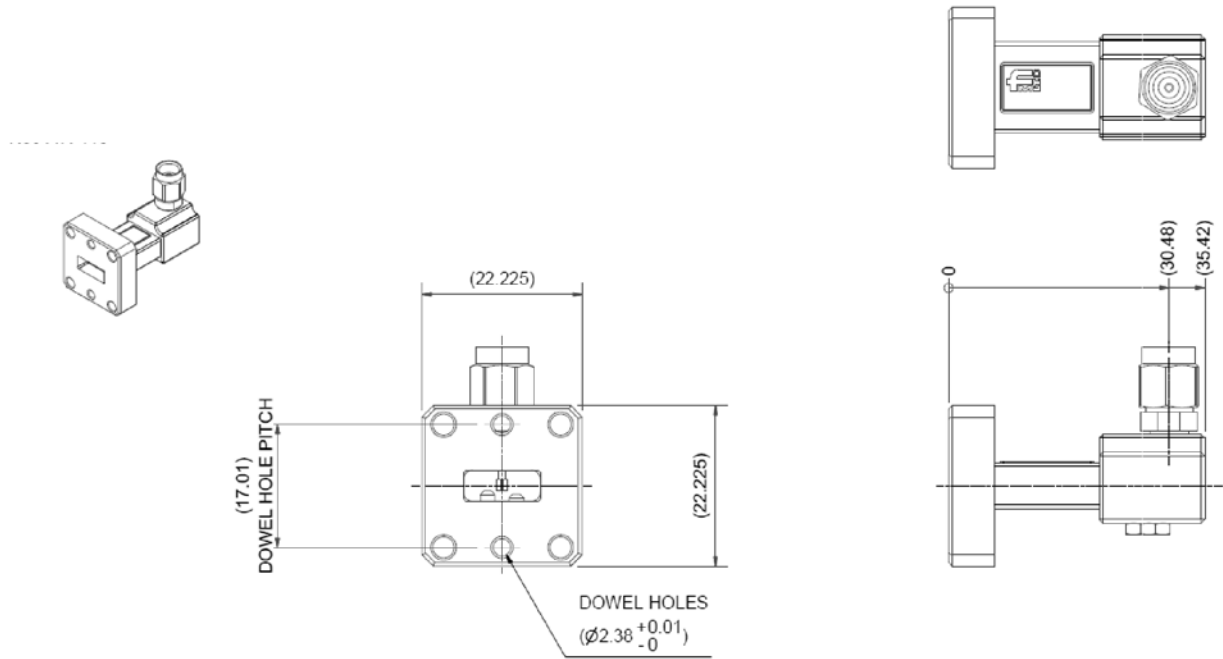


N9911_002_211

Termination Dimensions


NOTE The dimensions shown in the following graphics are in millimeters.

Figure 5-17 Termination, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-111

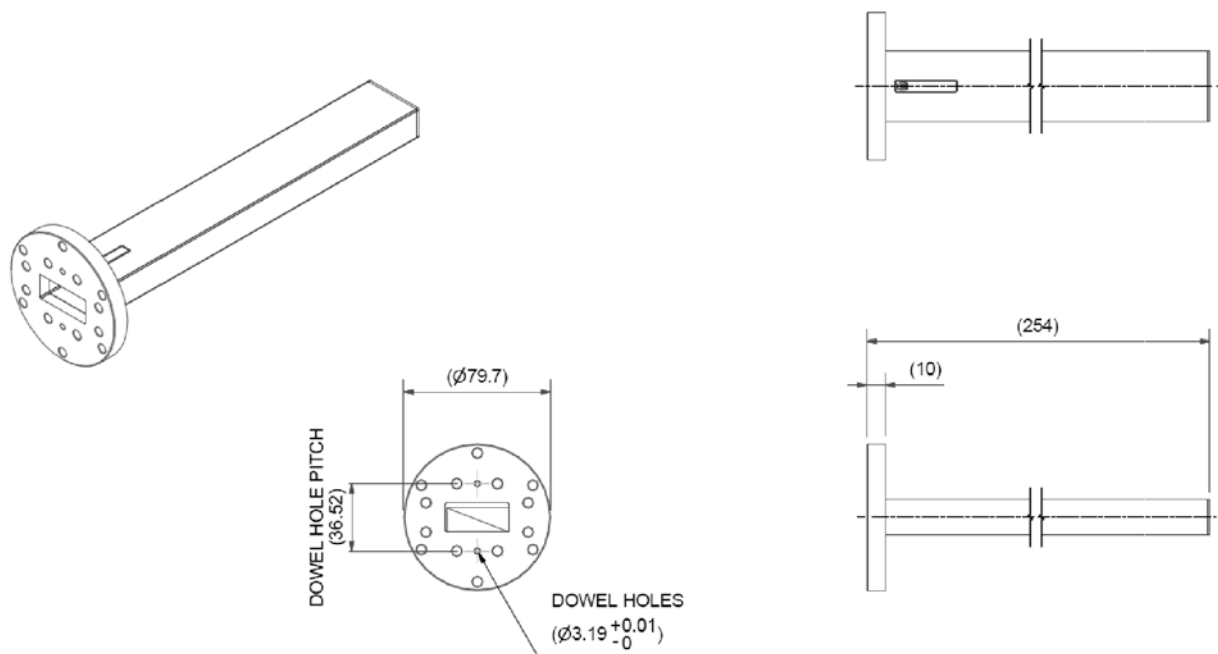


N9911_002_236

Figure 5-18 Termination, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-116

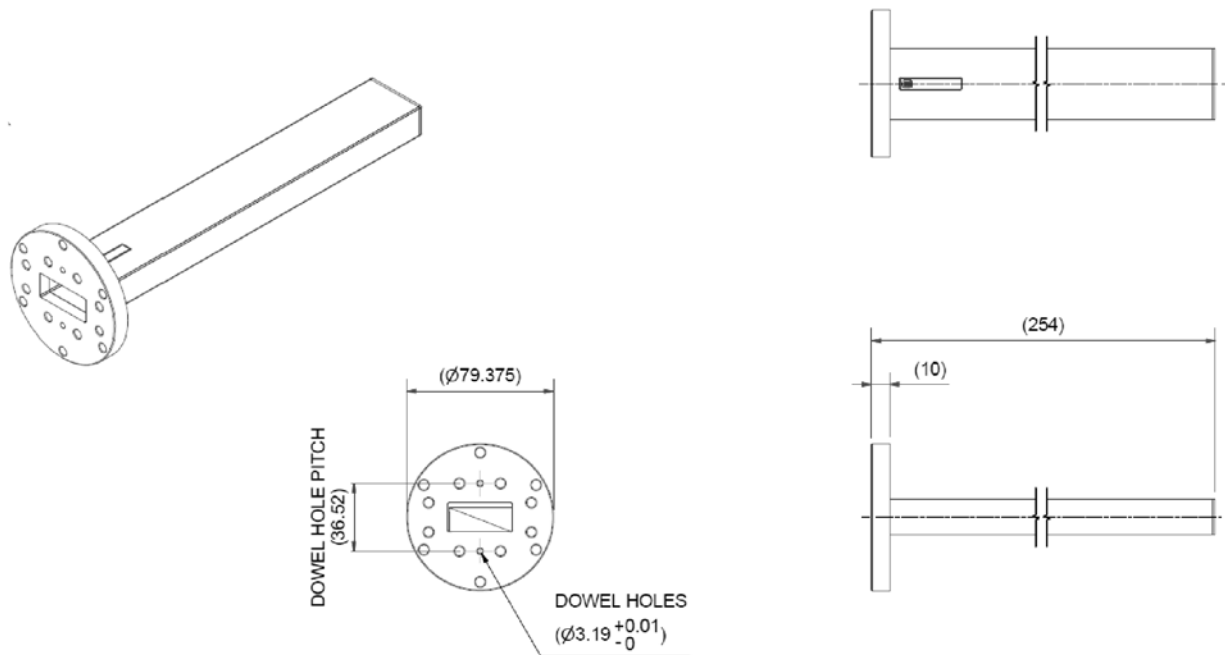


N9911_002_237

Figure 5-19 Termination, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-211

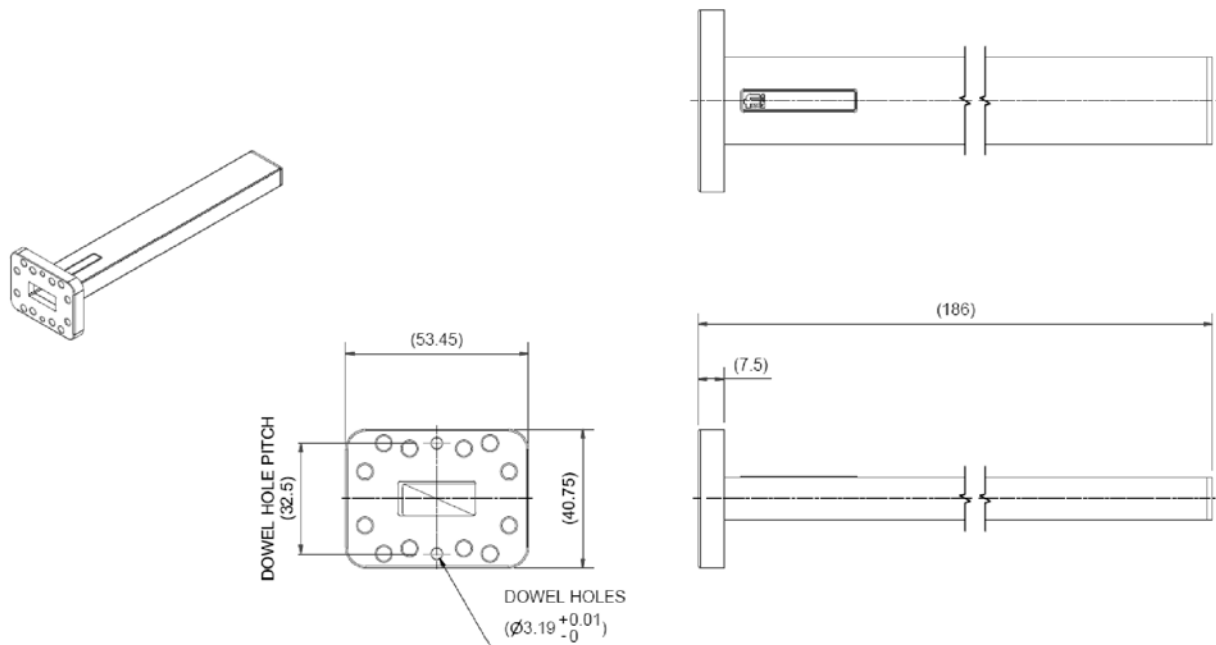


N9911_002_220

Figure 5-20 Termination, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-216

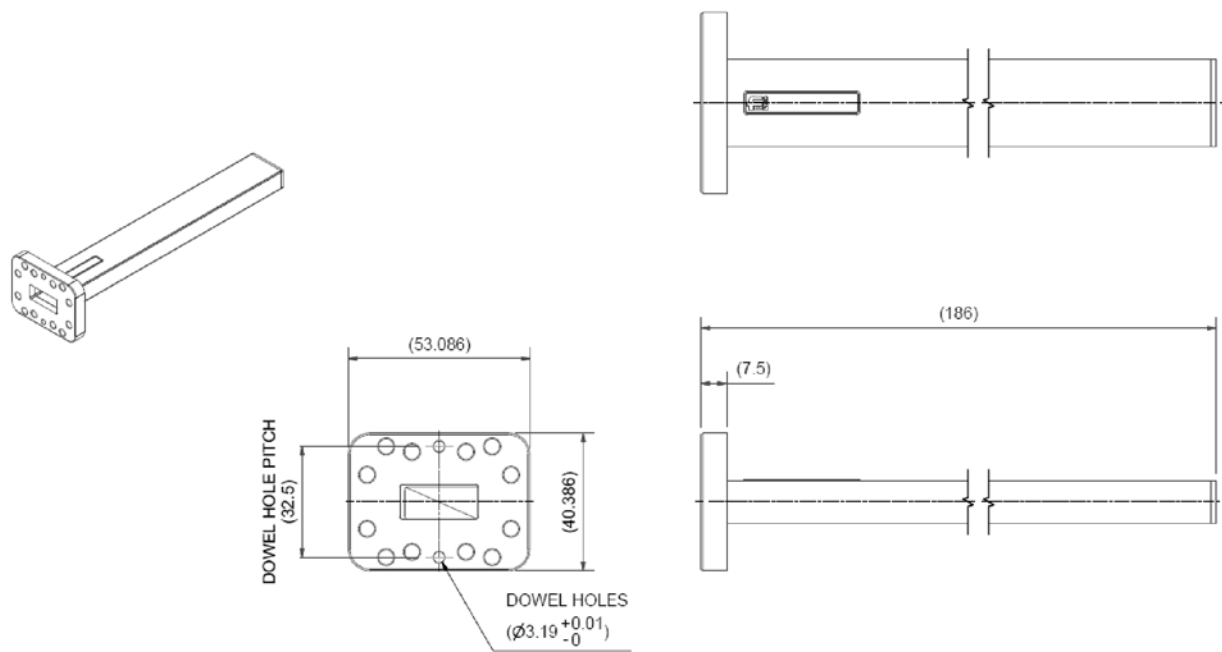


N9911_002_219

Figure 5-21 Termination, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-311

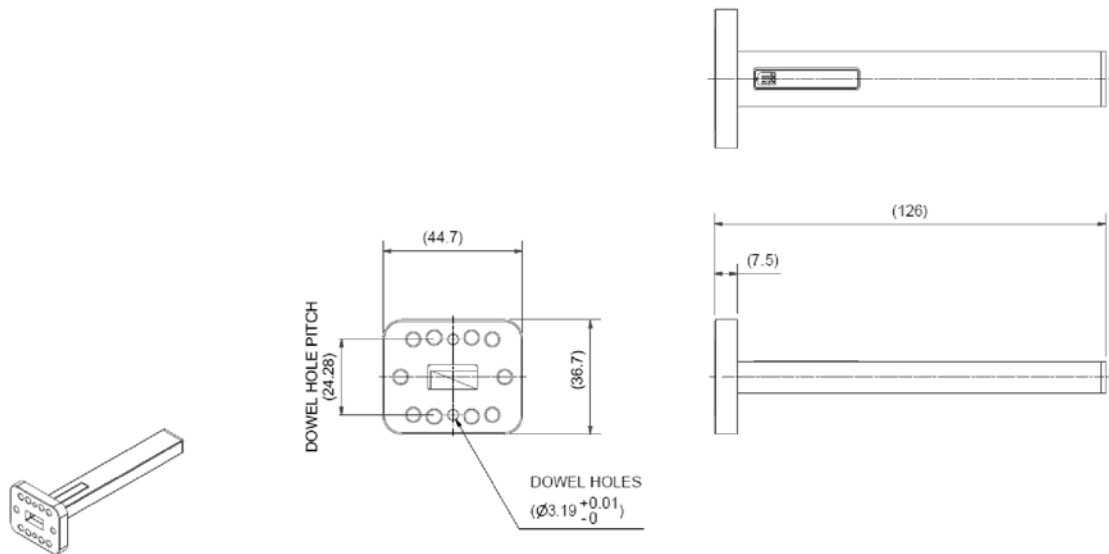


N9911_002_218

Figure 5-22 Termination, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-316

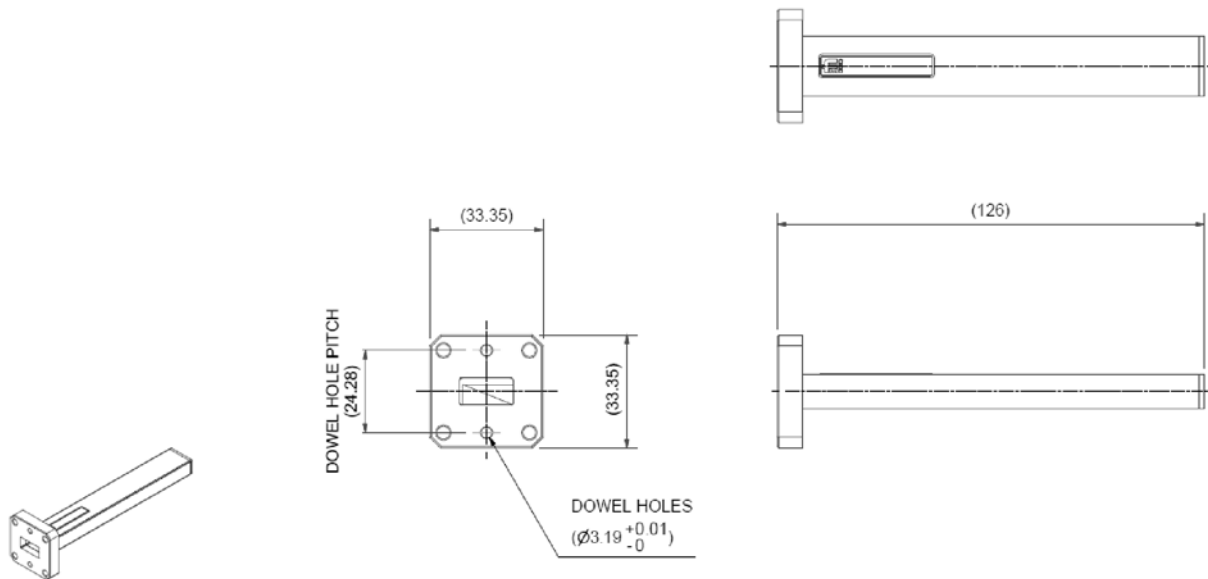


N9911_002_217

Figure 5-23 Termination, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-411

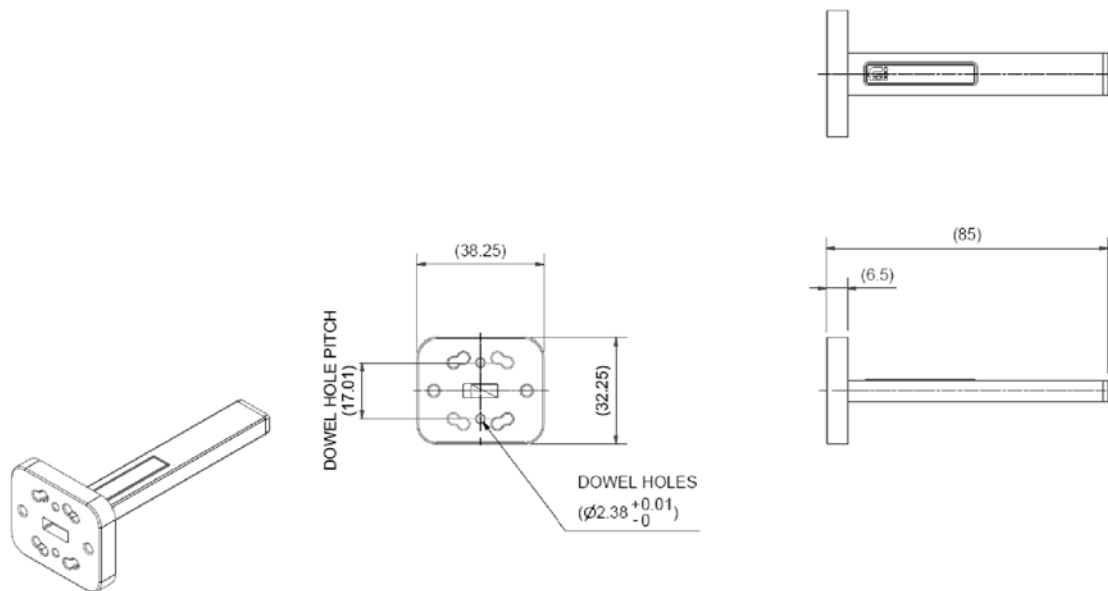

N9911_002_216

Figure 5-24 Termination, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-416

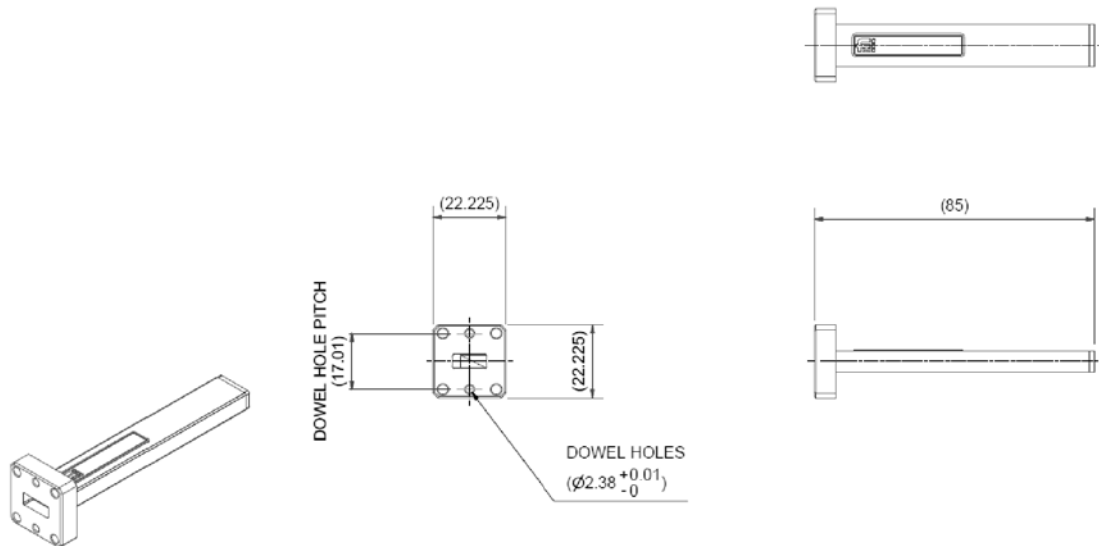


N9911_002_215

Offset Shim Dimensions


NOTE The dimensions shown in the following graphics are in millimeters.

Figure 5-25 Offset Shim, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-113

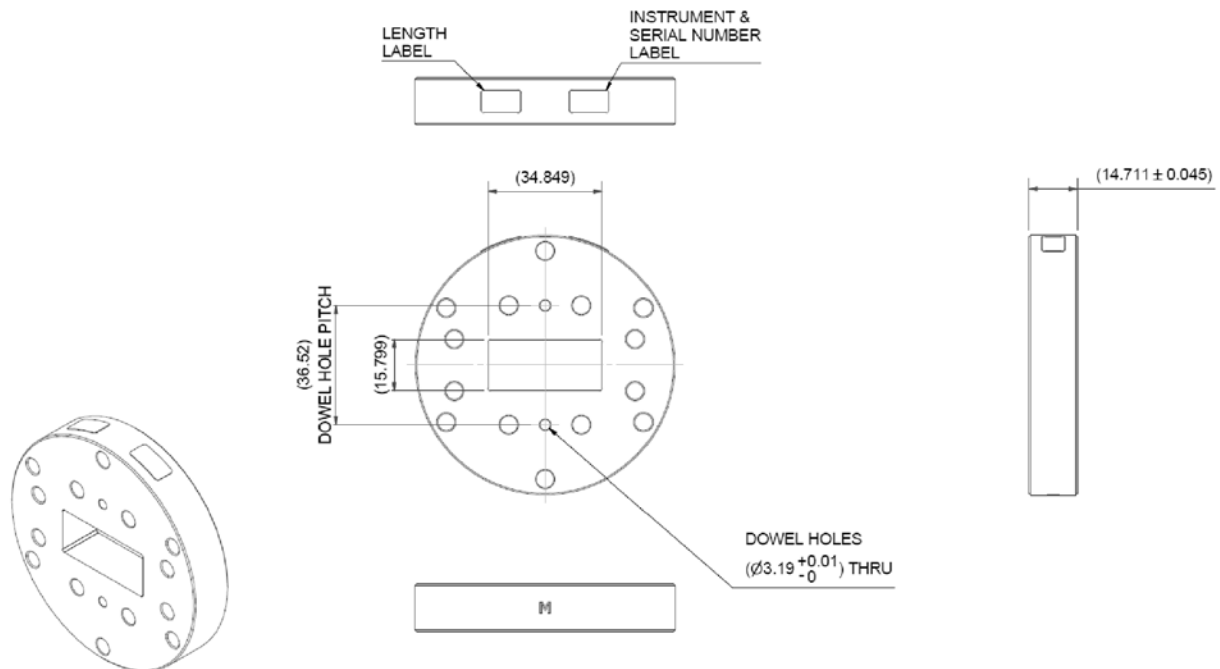


N9911_002_238

Figure 5-26 Offset Shim, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-118

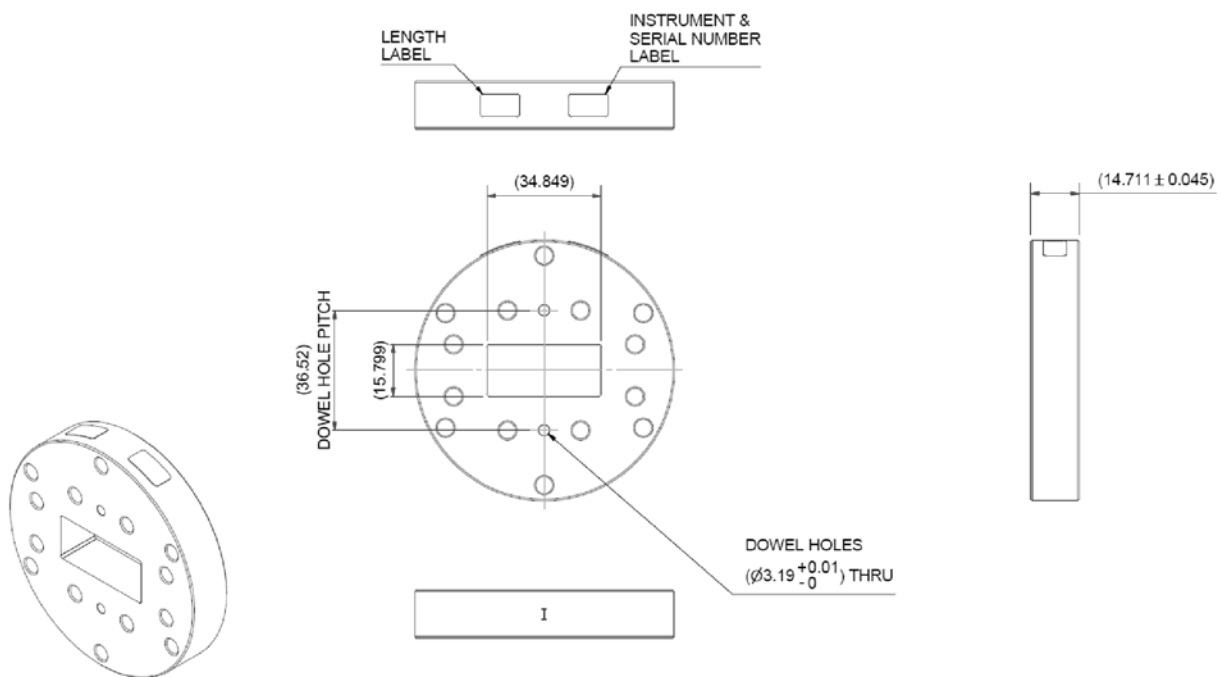


N9911_002_239

Figure 5-27 Offset Shim, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-213

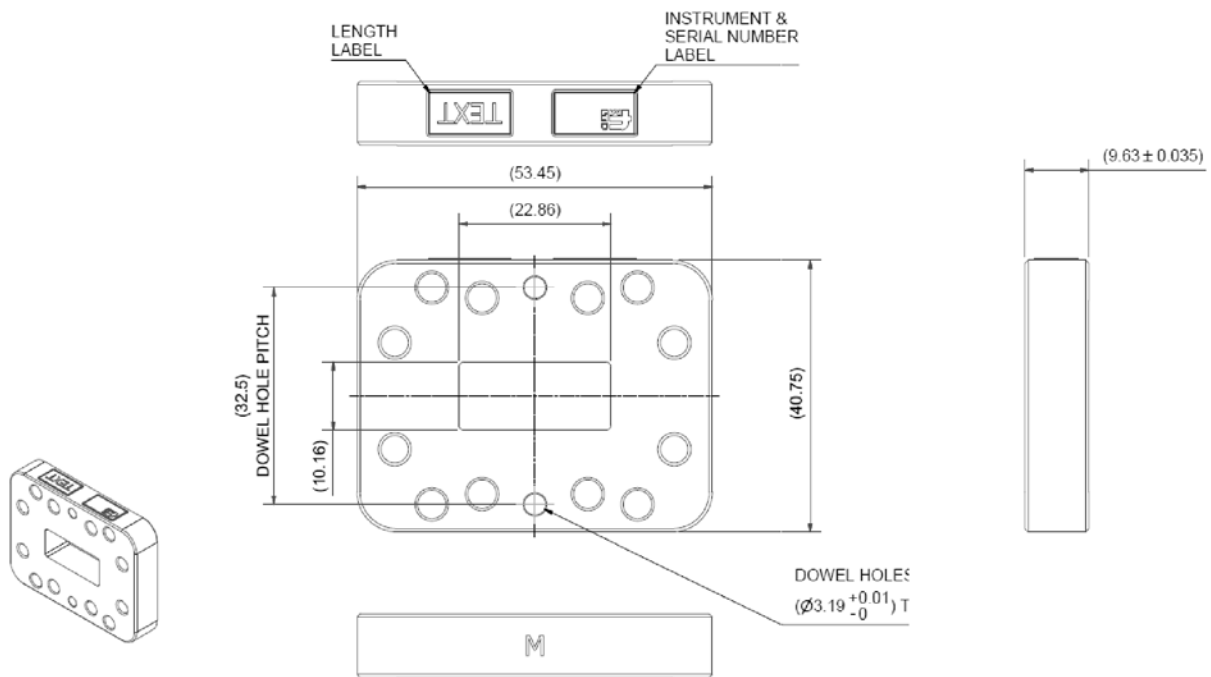


N9911_002_225

Figure 5-28 Offset Shim, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-218

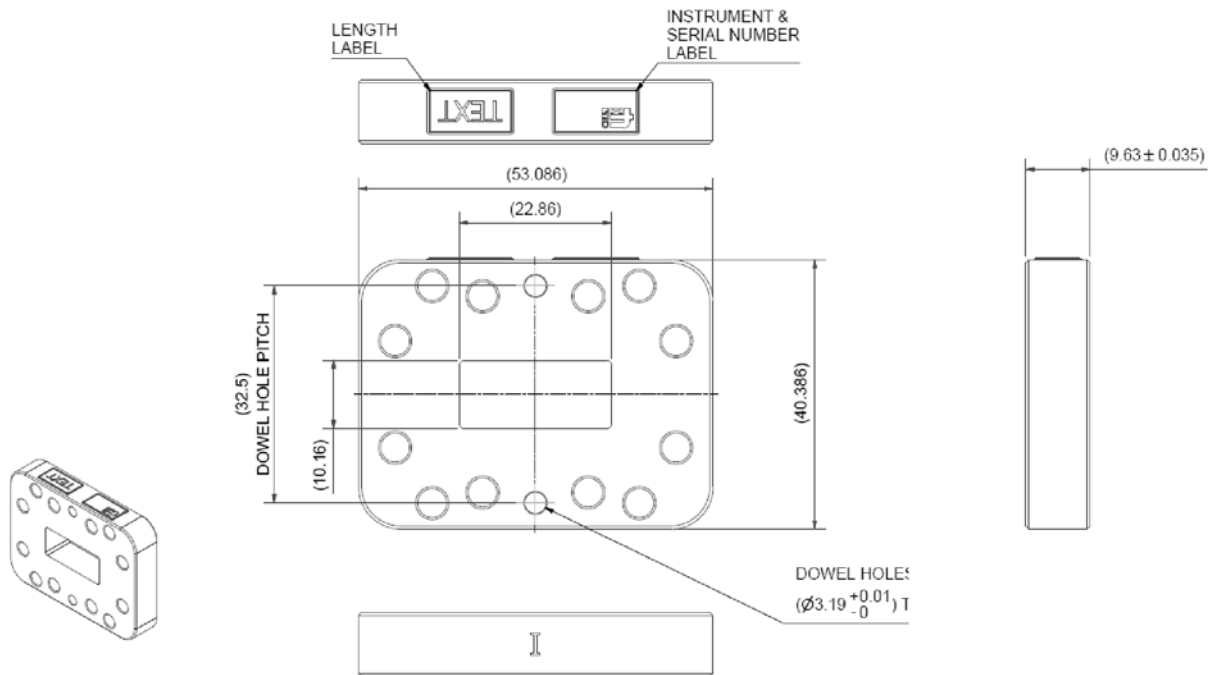


N9911_002_224

Figure 5-29 Offset Shim, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-313

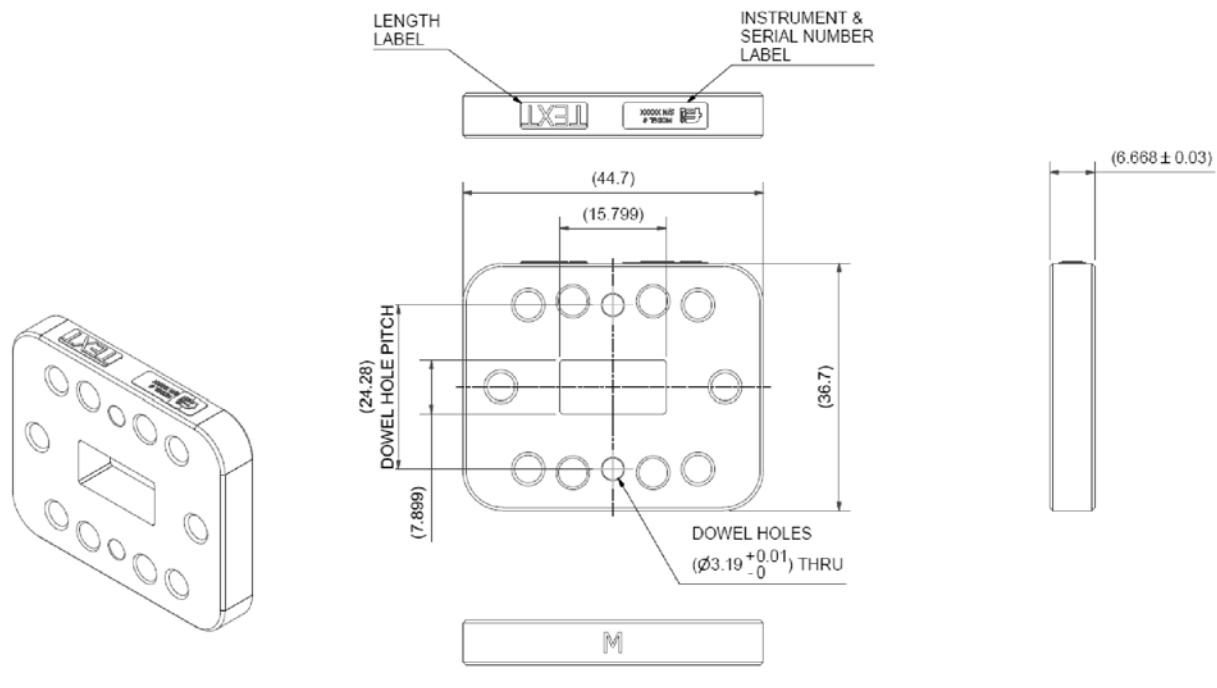


N9911_002_223

Figure 5-30 Offset Shim, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-318

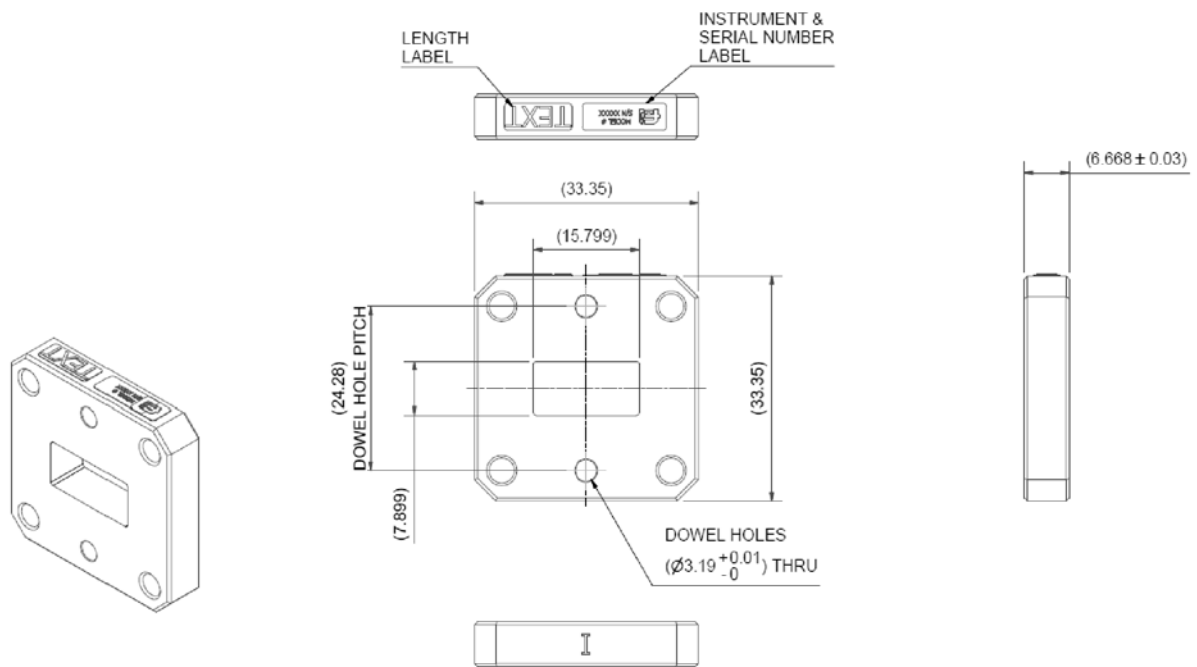


N9911_002_222

Figure 5-31 Offset Shim, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-413

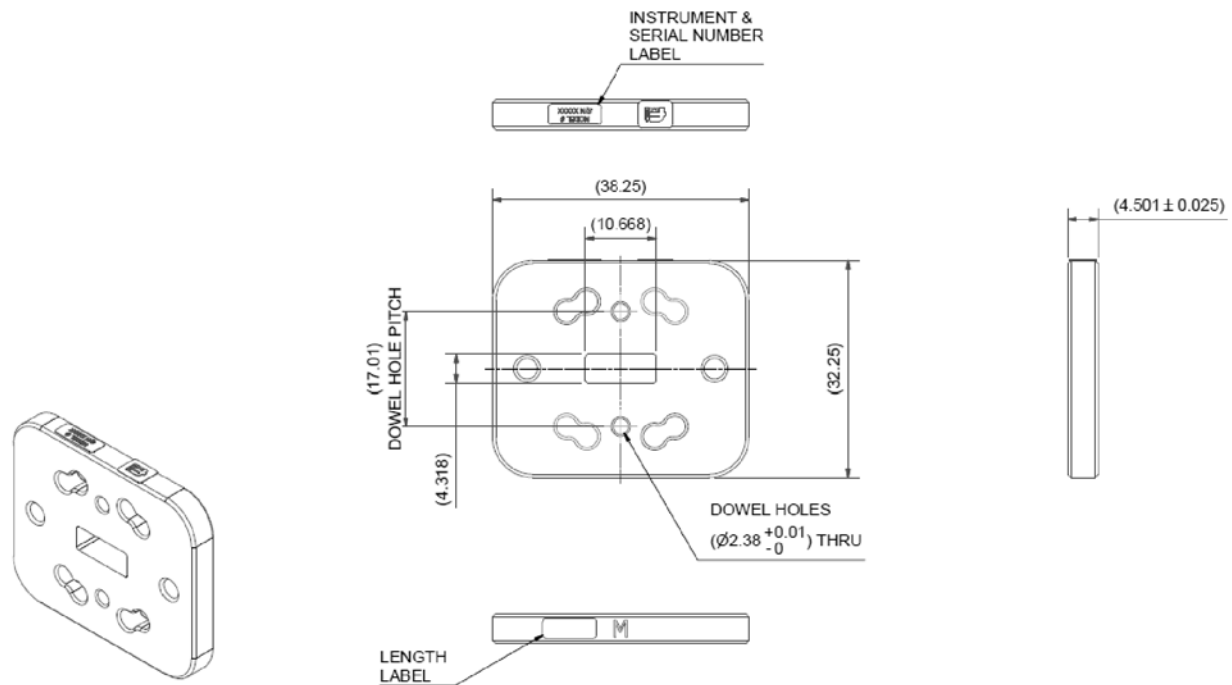

N9911_002_210

Figure 5-32 Offset Shim, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-418

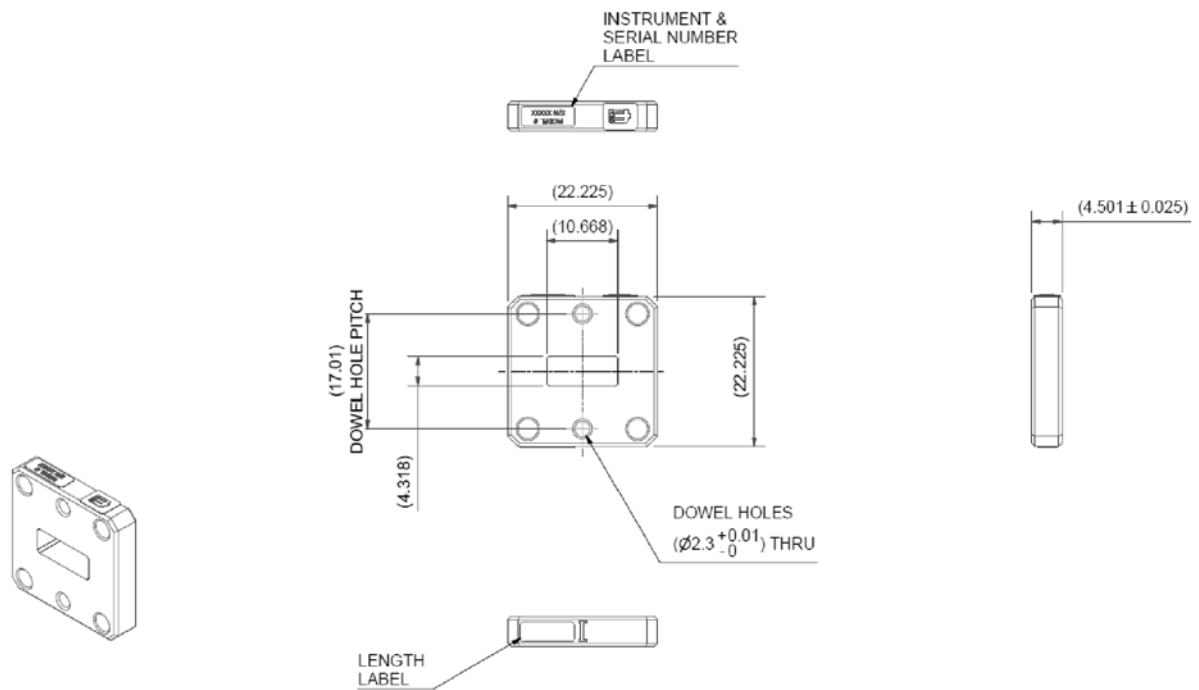


N9911_002_221

Flush Short Dimensions


NOTE The dimensions shown in the following graphics are in millimeters.

Figure 5-33 Flush Short, Waveguide Designators C-Band/WR137/WG14, Metric, Keysight Part Number N9911X-112

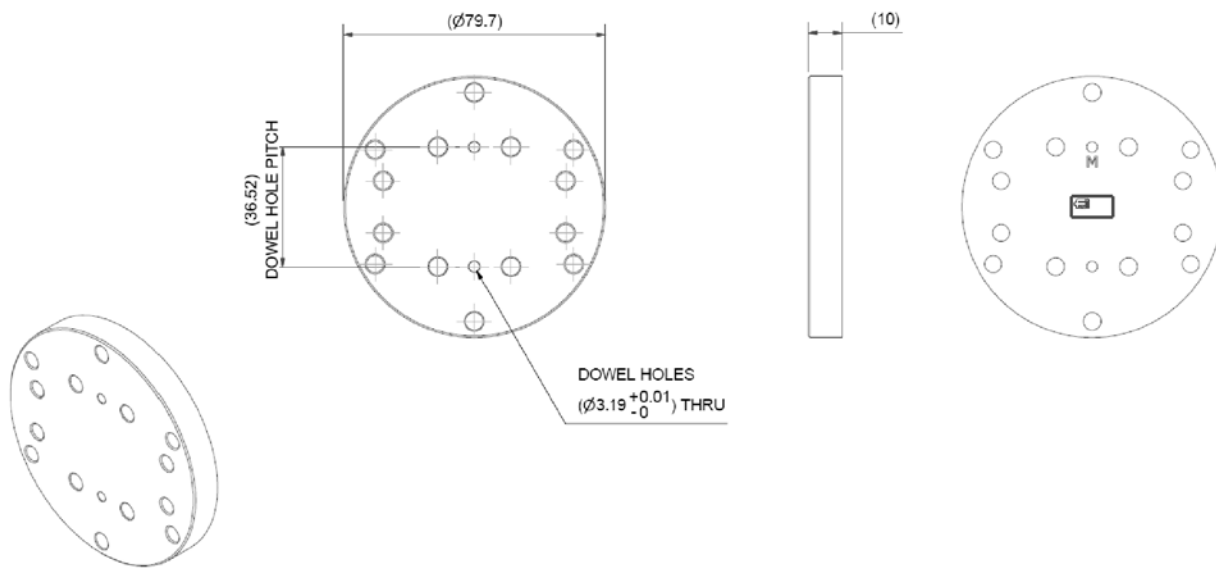

N9911_002_240


Figure 5-34 Flush Short, Waveguide Designators C-Band/WR137/WG14, English (Imperial), Keysight Part Number N9911X-117

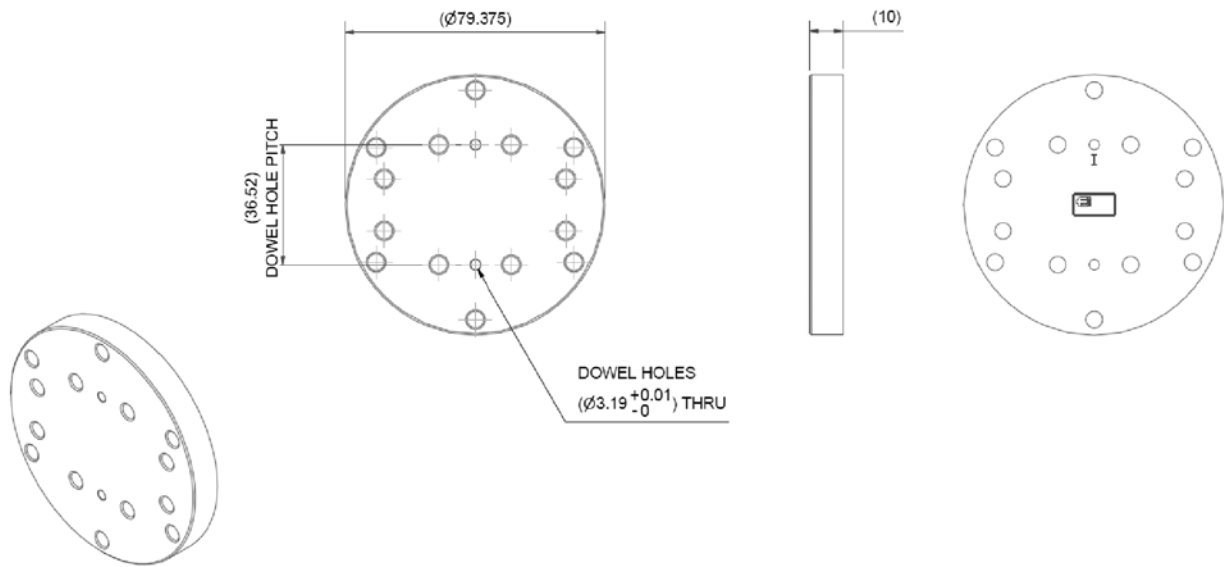

N9911_002_241


Component Dimensions
Flush Short Dimensions

Figure 5-35 Flush Short, Waveguide Designators X-Band/WR90/WG16, Metric, Keysight Part Number N9911X-212

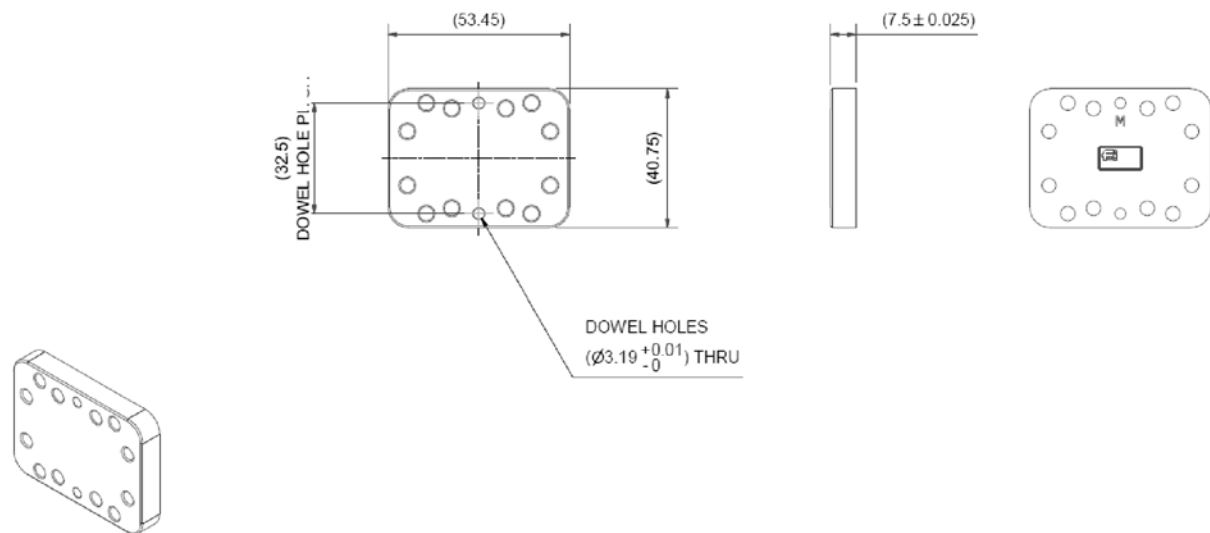


N9911_002_231

Figure 5-36 Flush Short, Waveguide Designators X-Band/WR90/WG16, English (Imperial), Keysight Part Number N9911X-217

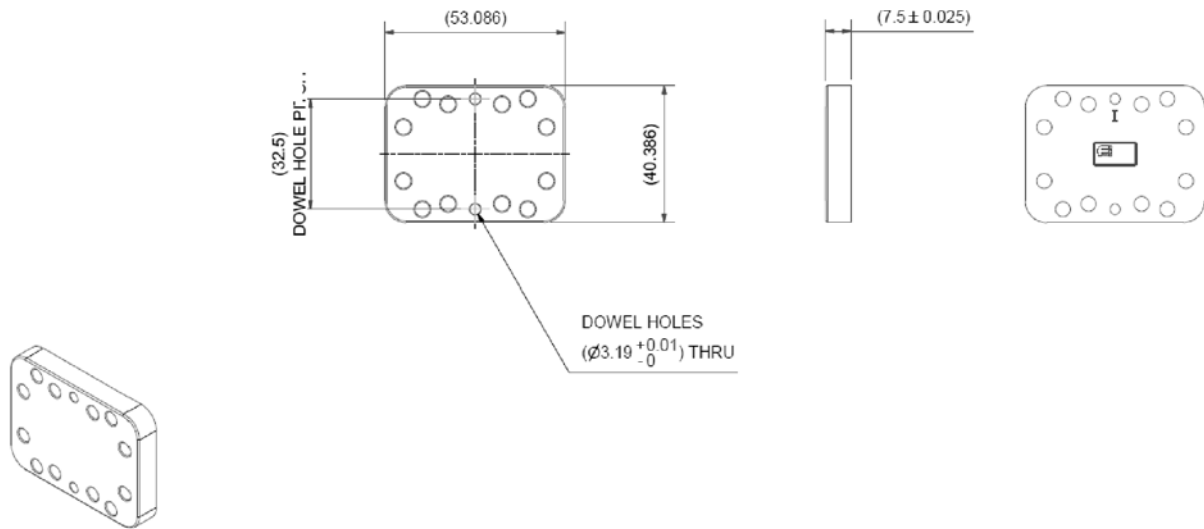


N9911_002_230

Figure 5-37 Flush Short, Waveguide Designators Ku-Band/WR62/WG18, Metric, Keysight Part Number N9911X-312

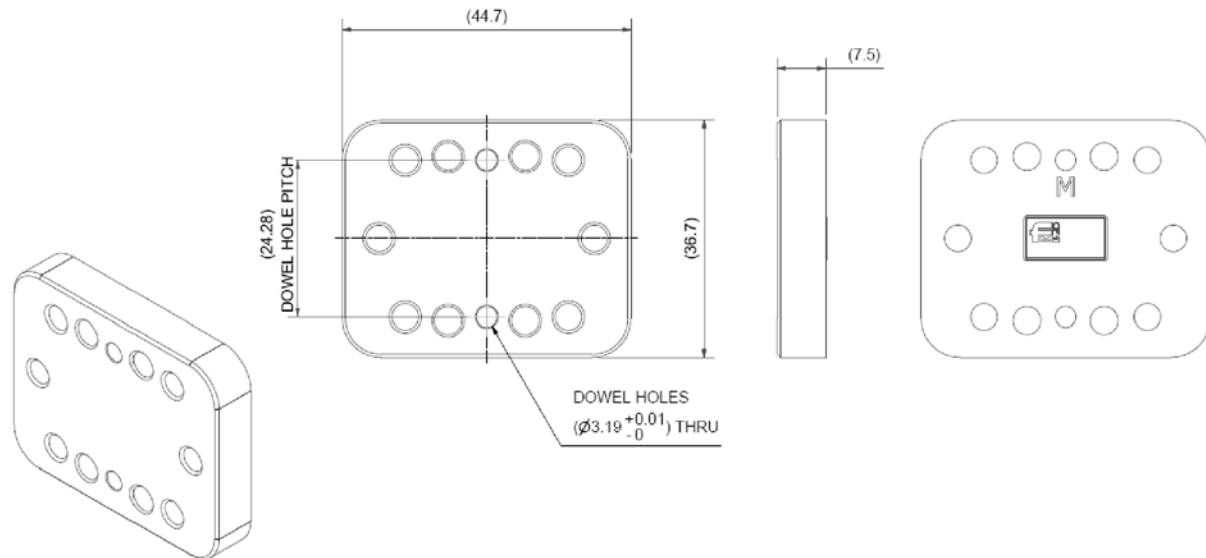

N9911_002_229


Figure 5-38 Flush Short, Waveguide Designators Ku-Band/WR62/WG18, English (Imperial), Keysight Part Number N9911X-317

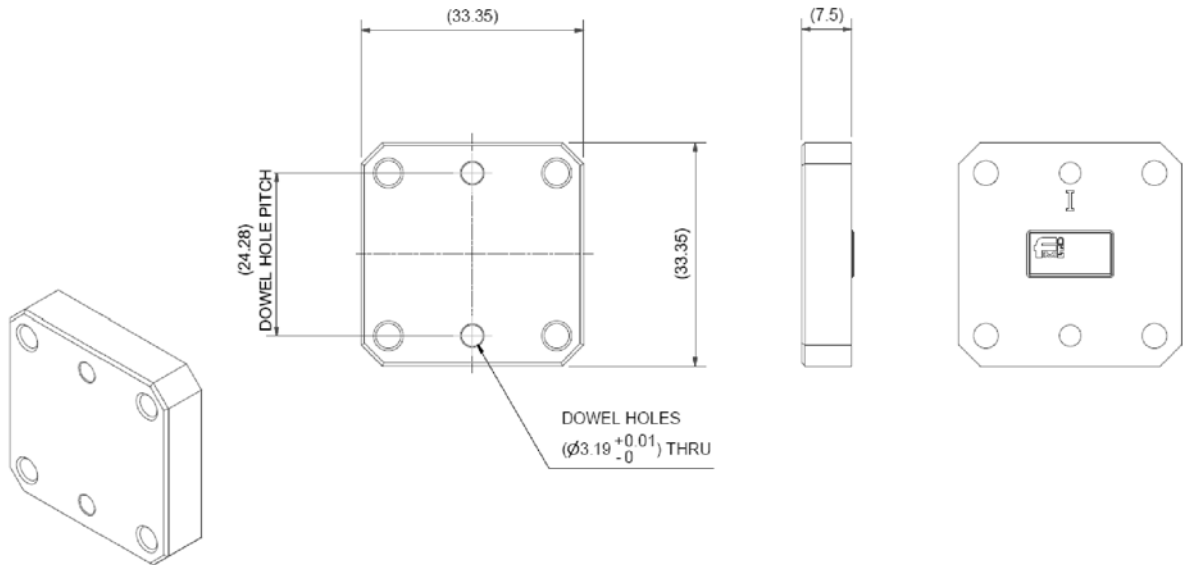

N9911_002_228


Component Dimensions
Flush Short Dimensions

Figure 5-39 Flush Short, Waveguide Designators K-Band/WR42/WG20, Metric, Keysight Part Number N9911X-412

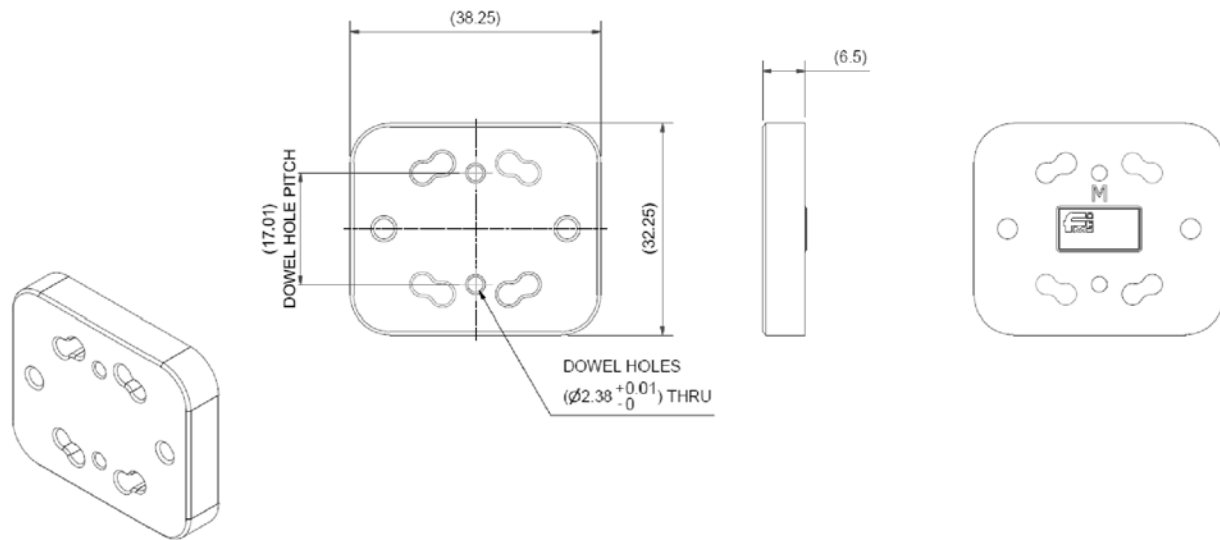

N9911_002_227

Figure 5-40 Flush Short, Waveguide Designators K-Band/WR42/WG20, English (Imperial), Keysight Part Number N9911X-417

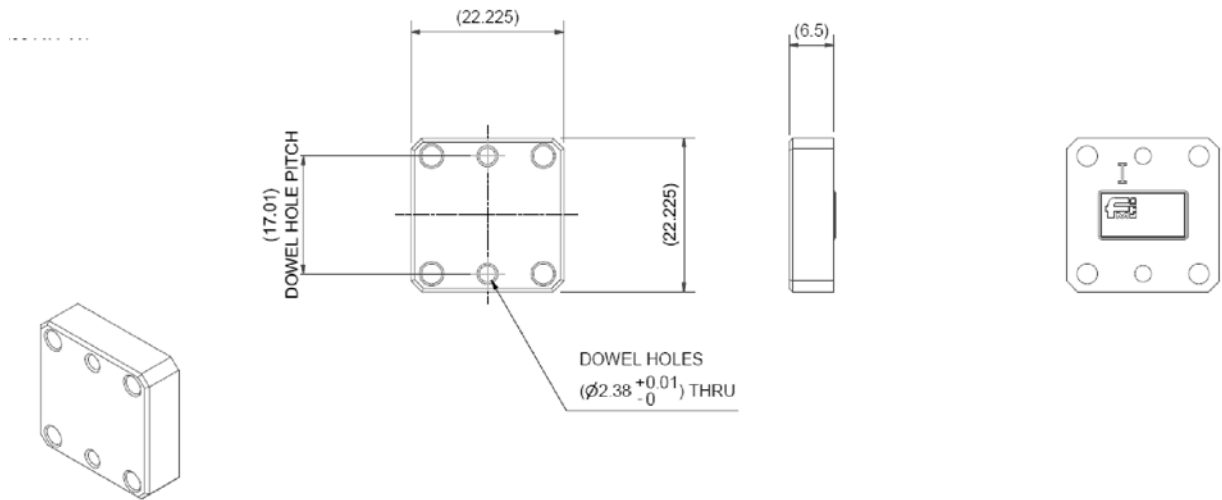

N9911_002_226

Component Dimensions
Flush Short Dimensions

A

- adapter
 - dimensions, 5-10
- alcohol, isopropyl
 - precautions for use of, 3-4
- aligning
 - precision flanges, 3-5
- assistance
 - contacting Keysight Technologies, 4-4

C

- calibration
 - bad, 4-2
 - components, overview, 1-2
 - frequency, 1-7
 - how to perform, 1-7
 - when to perform, 1-7
- cleaning
 - connectors, 3-4
 - mating plane surfaces, 3-4
- component
 - adapter, 3-8
 - adapter, waveguide-to-coax, 3-8, 3-9
 - cleaning, 3-4
 - connecting, 3-5
 - dimensions, 5-1
 - flush short, 3-8, 3-9
 - handling, 3-10
 - maintenance, 1-7
 - offset shim, 3-8
 - overview, 1-2
 - performance
 - failure, 4-2
 - serial number, record, 1-3
 - specifications
 - electrical, 2-5
 - storage, 3-10
 - temperature, 2-2
 - termination, 3-8
 - typical VSWR values, 2-3
 - visual inspection, 3-3
- compressed air
 - for cleaning, 3-4
- connecting
 - flanges, 3-5, 3-7
 - flush short to adapter, 3-9
 - for ESD protection, 3-2
 - offset shim between short and adapter, 3-8
 - termination to adapter, 3-8
- connector
 - cleaning, 3-4
 - mating plane surfaces, 3-4
- contacting Keysight Technologies, 4-3, 4-4

D

- damage
 - caused by electrostatic discharge, 3-2
- deviation from nominal phase, 2-5
- dimensions
 - adapter, 5-10
 - flange, 5-5
 - flush short, 5-34
 - offset shim, 5-26
 - shim, 5-26
 - short, 5-34
 - specifications, 2-5
 - termination, 5-18

E

- electrical
 - characteristics, effects of temperature, 2-2
 - specifications, 2-5
 - typical VSWR values, 2-3
- electrostatic discharge, *See* ESD
- environmental
 - regulations, 3-4
 - requirements, 2-2
- ESD
 - protection, 3-2

F

- flange
 - connect, 3-7
 - dimensions, 5-5
- flowchart, troubleshooting, 4-2
- flush short
 - dimensions, 5-34
- frequency
 - of calibration, 1-7
 - specification, 2-5

G

- general information, 1-1

H

- handling, 3-10
- how often to calibrate, 1-7
- how to calibrate, 1-7

I

- inspection
 - flange connection, 3-7
 - visual, 3-3
- instrument interface specifications, 2-4
- isopropyl alcohol
 - precautions for use of, 3-4

K

- Keysight Technologies
 - contacting, 4-3, 4-4

L

- load, *See* termination

M

- maintenance, preventive, 1-7
- mat, for ESD protection, 3-2
- mating plane surfaces
 - cleaning, 3-4
 - connector, 3-4

N

- nitrogen, for cleaning, 3-4
- numbers, serial, 1-3

O

- offset shim
 - dimensions, 5-26
- offset short, creating, 3-8
- oxygen, 3-4

P

- performance, verification, 4-2
- precision flanges, 3-5
- preventive maintenance, 1-7
- procedures
 - aligning flanges, 3-5
 - cleaning, 3-4
 - tightening flanges, 3-7

R

- recording component serial numbers, 1-3
- regulations, environmental, 3-4
- requirements
 - environmental, 2-2
 - temperature, 2-2
- return component to Keysight, 4-3
- return loss specification, 2-5

S

- serial numbers, 1-3
- service, 4-3
- shim dimensions, 5-26
- short
 - dimensions, 5-34
 - part numbers, 1-3, 1-4, 1-5, 1-6
- specifications, 2-1
 - characteristics, 2-5
 - component, 2-5
 - deviation from nominal phase, 2-5

- dimension, 2-5
- electrical, 2-5
- frequency, 2-5
- instrument interface, 2-4
- return loss, 2-5
- static electricity, 3-2
- storage, 3-10

T

- table mat, for ESD protection, 3-2
- temperature
 - cautions about, 2-2
 - requirements, 2-2
- termination
 - dimensions, 5-18
- troubleshooting, flowchart, 4-2
- typical VSWR values
 - component, 2-3

V

- visual inspection, 3-3
- VSWR typical values, 2-3

W

- when to calibrate the analyzer, 1-7
- wrist strap, for ESD protection, 3-2