
# D9010BJCC 100GBASE-CR4 Test Application



METHODS OF IMPLEMENTATION

# Notices

#### © Keysight Technologies 2014-2024

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies as governed by United States and international copyright laws.

### Trademarks

UNIX is a registered trademark of UNIX System Laboratories in the U.S.A. and other countries. Target is copyrighted by Thru-Put Systems, Inc.

#### Version

Version 3.70.20.0

Edition

#### April 2024

Available in electronic format only

#### Keysight Technologies, Inc. 1900 Garden of the Gods Road Colorado Springs, CO 80907 USA

## Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW. KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE

# TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

#### **Technology Licenses**

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

# U.S. Government Rights

The Software is "commercial computer software," as defined by Federal Acquisition Regulation ("FAR") 2.101. Pursuant to FAR 12.212 and 27.405-3 and Department of Defense FAR Supplement ("DFARS") 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public. Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at http://www.keysight.com/find/sweula. The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight: (1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release, perform, display, or disclose commercial computer software or commercial computer software documentation. No additional government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no

greater than Limited Rights as defined in FAR 27.401 or DFAR 227.7103-5 (c), as applicable in any technical data.

## Safety Notices

# CAUTION

A CAUTION notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

# WARNING

A WARNING notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

# Contents

# 1 Overview

100GBASE-CR4 Automated Testing–At a Glance / 8 Required Equipment and Software / 9 Hardware / 9 Software / 9 Licensing information / 9

# 2 Installing the Test Application and Licenses

Installing the Test Application / 12 Installing the License Key / 13 Using Keysight License Manager 5 / 13 Using Keysight License Manager 6 / 14

## 3 Preparing to Take Measurements

Calibrating the Oscilloscope / 18 Starting the 100GBASE-CR4 Test Application / 19 Configuring 100GBASE-CR4 Test Application for Test Runs / 23 Configuring Switch Matrix / 27 Overview / 27 Enabling Switch Matrix / 27 Establishing Connection to the Switch Drivers / 28 Configuring Signal Paths / 34 Configuring Signal Paths with Automatic Selection / 35 Configuring Signal Paths with Manual Selection / 35 Response Correction / 36

### 4 Main Voltage Measurements

Differential Peak to Peak Output Voltage Test with TX Disabled / 41 DC Common Mode Output Voltage Test / 42 AC Common Mode Output Voltage Test / 43 Differential Peak to Peak Output Voltage Test / 44

#### 5 Jitter and Signaling Rate Measurements

Signaling Rate / 47

Jitter (Even-Odd Jitter, Bounded Uncorrelated Jitter, Total Uncorrelated Jitter) / 48

# 6 Output Waveform Measurements

Steady State Voltage Vf / 51 Linear Fit Pulse Peak / 52 Signal-to-Noise-and-Distortion Ratio / 53

## 7 Normalized Coefficient Step Size Measurements

abs Coefficient Step Size c(1)inc c(0)hold c(-1)hold / 57abs Coefficient Step Size c(1)dec c(0)hold c(-1)hold / 58abs Coefficient Step Size c(1)hold c(0)inc c(-1)hold / 59abs Coefficient Step Size c(1)hold c(0)dec c(-1)hold / 60abs Coefficient Step Size c(1)hold c(0)hold c(-1)inc / 61abs Coefficient Step Size c(1)hold c(0)hold c(-1)dec / 62

# 8 Full Scale Range Tests

Minimum Pre-cursor Full-scale Ratio / 65 Minimum Post-cursor Full-scale Ratio / 66

### 9 Coefficient Initialization Measurements

Coefficient Initialization (c(0)+c(1)-c(-1))/(c(0)+c(1)+c(-1)) / 69 Coefficient Initialization (c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1)) / 70

## 10 Return Loss PNA/ENA Measurements

### 11 DME/EEE Waveform Measurements

DME Differential Peak-to-Peak Output Voltage Test / 75 DME T1-Transition Position Spacing (period) Test / 76 DME T2-Clock Transition to Clock Transition Test / 77 DME T3-Clock Transition to Data Transition Test / 78 EEE Differential Peak-to-Peak Output Voltage Test with TX Disabled / 79 EEE Differential Peak-to-Peak Output Voltage Test / 80 EEE Common Mode Deviation Voltage Test / 81

# 12 Exporting Measurement Results to Repository

Uploading Results to Repository / 84 KS6800A Series Analytics Service Software / 92

# 13 Debug Mode

Index

Keysight D9010BJCC 100GBASE-CR4 Test Application Methods of Implementation

# 1 Overview

100GBASE-CR4 Automated Testing—At a Glance 8 Required Equipment and Software 9



# 100GBASE-CR4 Automated Testing-At a Glance

The Keysight D9010BJCC 100GBASE-CR4 Test Application is an Ethernet test solution that covers the electrical timing parameters for 100GBASE-CR4 specification (IEEE 802.3bj D3p0).

The Keysight D9010BJCC 100GBASE-CR4 Test Application:

- Lets you select individual or multiple tests to run.
- Lets you identify the device being tested and its configuration.
- · Shows you how to make oscilloscope connections to the device under test.
- · Automatically checks for proper oscilloscope configuration.
- · Automatically sets up the oscilloscope for each test.
- Provides detailed information for each test that has been run and lets you specify the thresholds at which marginal or critical warnings appear.
- Creates a printable HTML report of the tests that have been run.

NOTE

The tests performed by the Keysight D9010BJCC 100GBASE-CR4 Test Application are intended to provide a quick check of the electrical health of the DUT. This testing is not a replacement for an exhaustive test validation plan.

#### Required Equipment and Software

In order to run the 100GBASE-CR4 automated tests, you need the following equipment and software:

#### Hardware

- Use one of the following Oscilloscope models. Refer to www.keysight.com for the respective bandwidth ranges.
  - Keysight Z-Series Oscilloscopes
  - Keysight UXR Oscilloscopes
- For differential probing (minimum 25GHz)

#### NOTE

# These can be used as an option, but will be BW limited. Instead, it is recommended to test with cables on the Real Edge channels.

- · N2802A 25 GHz InfiniiMax III Series probe amplifier
- · N2803A 30 GHz InfiniiMax III Series probe amplifier
- N2836A InfiniiMax III 26 GHz solder-in probe head
- For single-ended probing
  - SMA cables that are able to support the 25 Gb speed
- Keyboard, qty = 1, (provided with the Keysight Infiniium oscilloscope)
- Mouse, qty = 1, (provided with the Keysight Infiniium oscilloscope)
- Keysight also recommends using a second monitor to view the test application.

#### Software

- The minimum version of Infiniium Oscilloscope Software (see the Keysight D9010BJCC 100GBASE-CR4 Test Application Release Notes)
- Keysight D9010BJCC 100GBASE-CR4 Test Application software

#### Licensing information

Refer to the *Data Sheet* pertaining to 100GBASE-CR4 Test Application to know about the licenses you must install along with other optional licenses. Visit "http://www.keysight.com/find/D9010BJCC" and in the web page's **Document Library** tab, you may view the associated Data Sheet.

To procure a license, you require the Host ID information that is displayed in the Keysight License Manager application installed on the same machine where you wish to install the license.

The licensing format for Keysight License Manager 6 differs from its predecessors. See "Installing the License Key" on page 13 to see the difference in installing a license key using either of the applications on your machine.

1 Overview

Keysight D9010BJCC 100GBASE-CR4 Test Application Methods of Implementation

# 2 Installing the Test Application and Licenses

Installing the Test Application 12 Installing the License Key 13

If you purchased the D9010BJCC 100GBASE-CR4 Test Application separate from your Infiniium oscilloscope, you must install the software and license key.



# Installing the Test Application

- 1 Make sure you have the minimum version of Infiniium Oscilloscope software (see the D9010BJCC release notes). To ensure that you have the minimum version, select Help > About Infiniium... from the main menu.
- 2 To obtain the 100GBASE-CR4 Test Application, go to Keysight website: "http://www.keysight.com/find/D9010BJCC".
- 3 In the web page's **Trials & Licenses** tab, click the **Details and Download** button to view instructions for downloading and installing the application software.

### Installing the License Key

To procure a license, you require the Host ID information that is displayed in the Keysight License Manager application installed on the same machine where you wish to install the license.

Using Keysight License Manager 5

To view and copy the Host ID from Keysight License Manager 5:

- 1 Launch Keysight License Manager on your machine, where you wish to run the Test Application and its features.
- 2 Copy the Host ID that appears on the top pane of the application. Note that x indicates numeric values.

	Keysig	nt License Manager	
▲ Conn		Licenses on <b>Example (</b> localhost) 🖒	
		Full computer name:msr.is.keysight.com	
ectio		Host ID: PCSERNO, JBXXXXXXX	
SUIC			

Figure 1 Viewing the Host ID information in Keysight License Manager 5

To install one of the procured licenses using Keysight License Manager 5 application,

- 1 Save the license files on the machine, where you wish to run the Test Application and its features.
- 2 Launch Keysight License Manager.
- 3 From the configuration menu, use one of the options to install each license file.

3 ? _ □ ×			
Why do I need these tools?			
Install License File	Ctrl+I		
Install License from Text	Ctrl+T		
View License Alerts	Ctrl+L		
Explore Transport URLs			
About Keysight License Manager			

Figure 2 Configuration menu options to install licenses on Keysight License Manager 5

For more information regarding installation of procured licenses on Keysight License Manager 5, refer to Keysight License Manager 5 Supporting Documentation.

Using Keysight License Manager 6

To view and copy the Host ID from Keysight License Manager 6:

- 1 Launch Keysight License Manager 6 on your machine, where you wish to run the Test Application and its features.
- 2 Copy the Host ID, which is the first set of alphanumeric value (as highlighted in Figure 3) that appears in the Environment tab of the application. Note that x indicates numeric values.

Keysight License	Manager 6	
Home	Licensing Version	= Keysight License Manager Ver: 6.0.3 Date: Nov 9 2018
<b>.</b>	Copyright	= © Keysight Technologies 2000-2018
Environment	AGILEESOFD SERVER CONFIG	
View licenses	AGILEESOFD_SERVER_LOGFILE	<u>C:\ProgramData\Keysight\Licensing\Log\server_log.txt</u>
	SERVER LICENSE FILE	
License usage	AGILEESOFD LICENSE FILE	= <u>C:\ProgramData\Keysight\Licensing\Licenses\Other;C:\ProgramData\Keysight</u>
	FLO_LICENSE_FILE	
Borrow license	KAL_LICENSE_FILE	
incense	AGILEESOFD_DEBUG_MODE	
	FLEXLM_TIMEOUT	
	Default Hostid	= xxxxadxxxxbe xxbaxeacexee
	Ethernet Address	= XXXXadXXXXbe XXbaXeaceXee
	DIID	
	Physical MAC Address	= xxxxadxxxxbe PHY_ETHER=xxbaxeacexee
	IP Address	= 127.0.0.1
	Computer/Hostname	
	Username	
	PATH	= C:\Program Files (x86)\Common Files\Intel\Shared Libraries\redist\intel6
	•	•
	Compact View	
		Refresh Gose Heir

Figure 3 Viewing the Host ID information in Keysight License Manager 6

To install one of the procured licenses using Keysight License Manager 6 application,

- 1 Save the license files on the machine, where you wish to run the Test Application and its features.
- 2 Launch Keysight License Manager 6.
- 3 From the Home tab, use one of the options to install each license file.

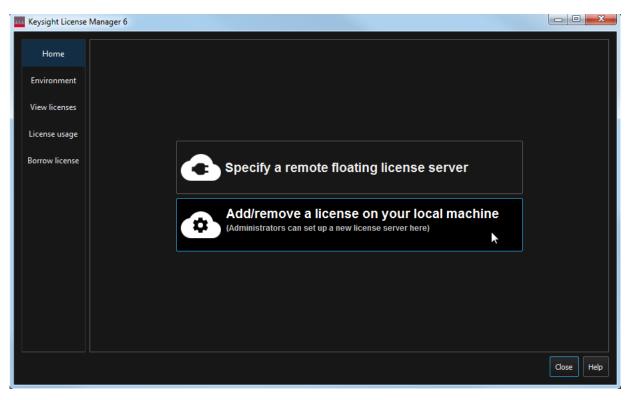


Figure 4 Home menu options to install licenses on Keysight License Manager 6

For more information regarding installation of procured licenses on Keysight License Manager 6, refer to Keysight License Manager 6 Supporting Documentation.

#### 2 Installing the Test Application and Licenses

Keysight D9010BJCC 100GBASE-CR4 Test Application Methods of Implementation

3

# Preparing to Take Measurements

Calibrating the Oscilloscope 18 Starting the 100GBASE-CR4 Test Application 19 Configuring 100GBASE-CR4 Test Application for Test Runs 23 Configuring Switch Matrix 27

Before running the automated tests, you should calibrate the oscilloscope and probe. No test fixture is required for this application. After the oscilloscope and probe have been calibrated, you are ready to start the 100GBASE-CR4 Test Application and perform the measurements.



# Calibrating the Oscilloscope

If you have not already calibrated the oscilloscope, refer to the *User Guide* for the respective Oscilloscope you are using.



If the ambient temperature changes more than 5 degrees Celsius from the calibration temperature, internal calibration should be performed again. The delta between the calibration temperature and the present operating temperature is shown in the **Utilities > Calibration** menu.



If you switch cables between channels or other Oscilloscopes, it is necessary to perform cable and probe calibration again. Keysight recommends that, once calibration is performed, you label the cables with the channel on which they were calibrated.

# Starting the 100GBASE-CR4 Test Application

- 1 Ensure that the 100GBASE-CR4 Device Under Test (DUT) is operating and set to desired test modes.
- 2 To start the 100GBASE-CR4 Test Application: From the Infiniium Oscilloscope's main menu, select **Analyze > Automated Test Apps > D9010BJCC 100GBASE-CR4 Test App**.
- Figure 5 shows the Keysight D9010BJCC 100GBASE-CR4 Test Application window as it appears when launched within the Infiniium application of the DSO Q-Series Oscilloscope. The Instrument Setup area in the Set Up tab displays Real Edge, which indicates Channels 1R and 3R on the oscilloscope.

🞽 100GBASE-CR4 Application 100GBASE-CR4 App Device 1					
File View Tools Help					
Set Up Select Tests Configure Connect Run Automate Results HTML Report					
Standard Option					
O 100GBASE-CR4 Multi-Lane Option					
O Single Lane					
Switch Matrix					
Instrument Setup					
Real Edge     Switch Matrix Setup					
Measurement Setup					
InfiniiSim Setup Set Channel Skew Saved Waveform Setup					
Test Report Comments (Optional)					
Device Identifier:					
Device User Description:					
Comments: You may enter information here to be included in the report.					
Connect PNA Connect ENA					
Messages					
Summaries (click for details) Details					
2021-05-16 11:07:18:034 PM Connected to The prima A Application initialized and ready for use.					
2021-05-16 11:07:21:696 PM Ready < ₩ →					
Unsaved Changes 0 Tests					

Figure 5 100GBASE-CR4 Test Application main window on a Z-Series Oscilloscope

• Figure 6 shows the Keysight D9010BJCC 100GBASE-CR4 Test Application window as it appears when launched within the Infiniium application of the UXR Oscilloscope. The Instrument Setup area in the Set Up tab displays the corresponding Channel assignments.

🞽 100GBASE-CR4 Application 100GBASE-CR4 App Device 1						
File View Tools Help	File View Tools Help					
Set Up Select Tests Configure Connect Run Automate Results HTML R	Report 🗸 🗸 🗸					
Standard Option						
O 100GBASE-CR4 Multi-Lane Option						
O Single Lane						
Switch Matrix						
Instrument Setup						
Channels 1 and 2 Switch Matrix Setup						
Channels 3 and 4						
Measurement Setup						
Infinition Cotum	ne Number e0 🔽					
Test Report Comments (Optional)						
Device Identifier:						
Device User Description:						
Comments: You may enter information here to be included in the report.						
Connect PNA Connect ENA						
Messages						
Summaries (click for details) Details						
2019-05-06 12:34:08:765 AM Ready Application initializ	zed and ready for use.					
0 Tests						

Figure 6 100GBASE-CR4 Test Application main window on a UXR Oscilloscope

Set Up	Lets you identify and set up the test environment, including information about the device under
001 Op	test.
	Standard Option Section
	It has 100 GBASE-CR4 radio button selected by default, you may select the lane options as
	Single Lane or Switch Matrix. When Switch Matrix is selected, the Switch Matrix Setup option
	is enabled in the <b>Instrument Setup</b> section.
	<ul> <li>Instrument Setup Section</li> </ul>
	In case of Digital Storage Oscilloscopes with real edge channels, the <b>Real Edge</b> option is selected by default. In case of a UXR Oscilloscope, you may select any one of the two options, that is, <b>Channel 1 and 2</b> or <b>Channel 3 and 4</b> . You may click <b>Switch Matrix Setup</b> option to
	configure the Switch Matrix for multi-lane testing. Optionally, Switch Matrix can also be configured from <b>Tools</b> menu > <b>Switch Matrix</b> option.
	Measurement Setup Section
	<ul> <li>InfiniiSim Setup button: This allows to setup InfiniiSim.</li> </ul>
	• Set Channel Skew button: This allows to visually adjust and skew the channels.
	<ul> <li>Saved Waveform Setup button: This allows to select the saved waveforms on which the application will run measurement tests.</li> </ul>
	<ul> <li>Select Lane Number button: This option allows to select one of the available lanes for topting that is lange lange lange or lange</li> </ul>
	testing, that is, Lane0, Lane1, Lane2, or Lane3. <ul> <li>Test Report Comments (Optional) Section</li> </ul>
	This section allows to add device related info which is printed in the final HTML report. It is
	quite helpful in easy identification of the specific DUTs in case of multi-DUT testing.
	• Device Identifier: This field allows to add a unique identifier for your device.
	<ul> <li>Device User Description: This field allows to provide a description of the DUT.</li> </ul>
	Comments: This is an additional field which allows a user to add descriptive information
	about the DUT or the measurement being carried out.
	<ul> <li>Connect PNA Button         This option allows to connect to a Performance Network Analyzer through following two mode:     </li> </ul>
	Enter/Select VISA address/alias (or SICL address)
	This field allows to enter/select the VISA or SICL address of a network instrument in order
	to connect to the specific instrument. <ul> <li>Select from Keysight Connection Expert 'My Instruments'</li> </ul>
	This field allows to select one of the instruments already connected through Keysight
	Connection Expert.
	Note: If a "No instrument found." message is displayed even though the instrument is
	visible on the Keysight Connection Expert. Please open the <b>Keysight Connection Expert</b>
	application, and select the particular instrument. Then, in the details section of the instrument, displayed in the right pane, please select the <b>Edit</b> icon to <b>Edit Settings for the LAN Instrument</b> . Then, please select the <b>Set Protocol</b> option as <b>Socket</b> and click <b>OK</b> .
	Connect ENA Button
	This option allows to connect to an Economy Network Analyzer through following two modes: • Enter/Select VISA address/alias (or SICL address)
	This field allows to enter/select the VISA or SICL address of a network instrument in order
	to connect to the specific instrument.
	Select from Keysight Connection Expert 'My Instruments'
	This field allows to select one of the instruments already connected through Keysight Connection Expert.
	Note: If a "No instrument found." message is displayed even though the instrument is visible on the Keysight Connection Expert. Please open the <b>Keysight Connection Expert</b>
	application, and select the particular instrument. Then, in the details section of the instrument, displayed in the right pane, please select the <b>Edit</b> icon to <b>Edit Settings for the</b>
	LAN Instrument. Then, please select the Set Protocol options as Instrument (VXI-11) and HiSlip, then click OK.
Select Tests	LAN Instrument. Then, please select the Set Protocol options as Instrument (VXI-11) and

The task flow pane and the tabs in the main pane show the steps you take in running the automated tests:

Connect	Shows you how to connect the oscilloscope to the device under test for the tests that are to be rul
Run	Starts the automated tests. If the connections to the device under test need to be changed while multiple tests are running, the tests pause, show you how to change the connection, and wait for you to confirm that the connections have been changed before continuing.
Automate	Lets you construct scripts of commands that drive execution of the application.
Results	Contains more detailed information about the tests that have been run. You can change the thresholds at which marginal or critical warnings appear.
HTML Report	Shows a compliance test report that can be printed.

NOTE

In the **Configure** tab, the values for all such Configuration parameters that are Oscilloscope-dependent, will correspond to the Oscilloscope Model (DSOs or UXRs), where you are running the Test Application.

#### Configuring 100GBASE-CR4 Test Application for Test Runs

To run one or more compliance tests on the DUT, which is connected to Oscilloscope, proceed to configure the 100GBASE-CR4 Test Application:

- In the Set Up tab (shown in Figure 5 and Figure 6), select a Multi-Lane Option to determine the lane where the tests must be performed for the 100GBASE-CR4 standard.
   If Switch Matrix is selected in the Multi-Lane Option, click Switch Matrix Setup to configure the Switch Matrix in the Test App. Refer to "Configuring Switch Matrix" on page 27 for more details.
- 2 In the Select Tests tab, select one or more tests.
- 3 In the **Configure** tab, you may change the values assigned to one or more options to cater to the compliance requirements for the selected tests. By default, the 100GBASE-CR4 Test Application sets optimum values for each configuration parameter.

🞽 100GBASE-CR4 Application 100GBASE-CR4 App Device 1					
File View Tools Help					
Set Up Select Tests Configure Connect Run Automate	Results HTML Report				
Mode: 🔘 Compliance 🔵 Debug					
<ul> <li>IEEE802.3 Tests         Signaling Rate (25.78125e9)         Number of UI (1e6)         TX On Voltage Scale (Auto)         TX Off Voltage Scale (Auto)         Disable Pattern Check (Enable)         Save Tested Waveforms (No)         Select Waveform Directory (C:\Temp\KRwfm)</li> </ul>	(Click on a setting to the left)				
Messages					
	Details				
2019-05-06 12:36:42:753 AM Exit?	Exit the application? [Response: Cancel (OKCancel)]				
0 Tests					

Figure 7 Configure tab in the 100GBASE-CR4 Test Application

4 In the Connect tab, view the instructions along with the connection digram to ensure that all requirements for the physical setup of the testing instruments and the DUT are met. Click Connection Completed to indicate to the Test Application that the required hardware setup is complete. The connection diagram for most of the tests matches the one shown in Figure 5 for DSO-Q Series Oscilloscopes and Figure 6 for UXR Series Oscilloscopes. However, it is a good

practice to verify the connection diagram and instructions displayed under this tab. The Test Application automatically indicates any changes in connections, if needed, during test runs.

5 Click **Run Tests** under this tab if you wish to start running tests. However, if you wish to modify the run settings before performing test runs, switch to the **Run** tab.

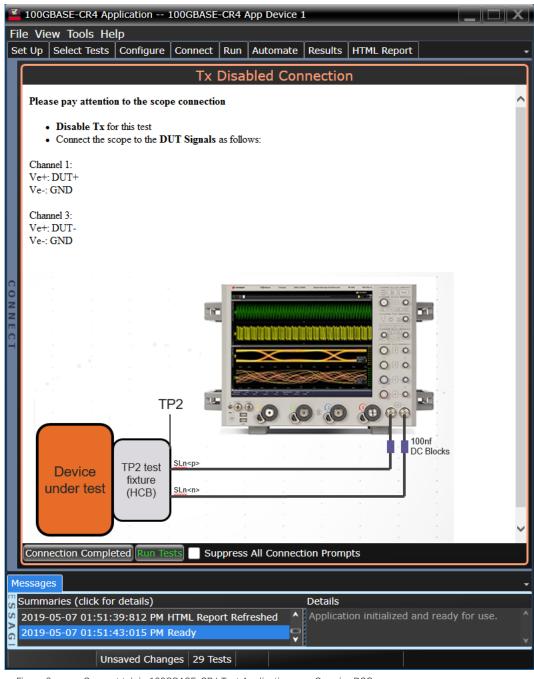


Figure 8 Connect tab in 100GBASE-CR4 Test Application on a Q-series DSO

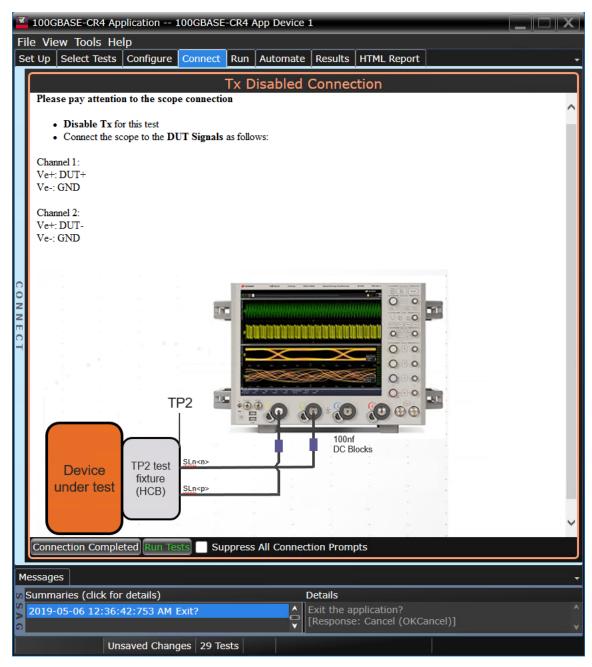


Figure 9 Connect tab in 100GBASE-CR4 Test Application on a UXR scope

- 6 In the **Run** tab, you may optionally modify one or more settings as described below, else click **Run** to start the test runs:
  - · determine the number of times each test must be run,
  - · automate specific actions in case of events,
  - store results for certain type of test trials only,
  - send email notifications if the test runs pause or stop during runs.

₹	🞽 100GBASE-KR4 Application 100GBASE-KR4 App Device 1					
File View Tools Help						
S	Set Up Select Tests Configure Connect Run Automate Results HTML Report					
RUN	Run     Pause       Sequencer       Run tests       Once       Event       Detect events       Store Mode       During run, store details for Worst       Trials (up to 25)					
	Email					
	Send email when run is paused or stopped					
	Summary: - Run tests once - Store details for up to 25 worst trials (margin)					
Messages 🗸						
Summaries (click for details) Details 2019-05-07 09:25:51:452 AM HTML Report Refreshed 2019-05-07 09:25:54:350 AM Ready vertical of the second seco						

Figure 10 Run tab in 100GBASE-CR4 Test Application

- 7 In the **Automate** tab, you may optionally configure automation scripts to perform specific actions/sequences within the Test Application.
- 8 In the **Results** tab, which appears automatically after test runs are complete, view the test results displayed for each selected test.
- 9 In the **HTML Report** tab, view a comprehensive report for each test within the Application. The Test Application enables exporting these results in CSV or HTML format for the purpose of analysis.

To perform a high-level analysis on each measurement data, you may upload the results to the KS6800A Series Analytics Services Software. Refer to "Uploading Results to Repository" on page 84 to understand an overview on the functionality of this feature.

#### Configuring Switch Matrix

Overview

Devices, with 100GBASE-CR4 standard, can run with the switch matrix using four dual single-ended connections or without the switch matrix using four differential probe connections. Both options are fully automated to switch across the four lanes. Switch Matrix requires either the Keysight U3020A S26 or the BitifEye BIT2100.

This chapter describes the switch matrix feature and steps for configuring the switch matrix in the Keysight D9010BJCC 100GBASE-CR4 Test Application.


An Oscilloscope has only four Channels to run tests. The limited number of channels may, at times, limit the testing of some multi-lane standards. Also, it may prove to be a hindrance to run test procedures for multi-port devices or simultaneous testing of multiple devices. The Switch Matrix feature on the Infiniium Oscilloscope overcomes such limitations.

The purpose of the 'Switch Matrix' feature is to ease the testing procedure, make it more feasible and to reduce the overall time. Using this feature, you can connect multiple lanes of the source devices to the correct switches and to obtain an accurate signal path whenever required.

Keysight recommends the following switches to be used with the Test Application:

- Keysight U3020A S26
- BitifEye BIT-2100

The following figure shows the connection setup for 100GBASE-CR4 tests with the switch matrix.

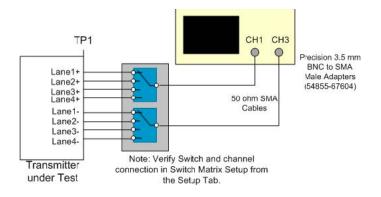

Enabling Switch Matrix

Before you begin the testing of multiple lane pairs of the source devices simultaneously, you must enable the Switch Matrix feature.

To enable the switch matrix feature:

1 Click Tools > Switch Matrix....

Tools Help	
Compliance Limits	۲
Infiniium	۲
Switch Matrix	

2 In the **Configure Switch Matrix Settings** dialog box, click **On** to enable the Switch Matrix feature.

ſ	Configure Switch Matrix Settings*
	C Off € On

Enabling the Switch Matrix feature also enables the automated switch control. The option **Automatically select drivers and paths (limited models)** in the **Configuration Mode** section of the **Controller** tab is selected by default.

Config	Configure Switch Matrix Settings*				
○ Off	• On				
Controller	Signal Paths Response Co	prection			
-	Configuration Mode				
C Manu	ally perform these tasks (ar	y supported model)			

Establishing Connection to the Switch Drivers

Establishing connection to the Switch Drivers – Automatically

In the Configure Switch Matrix Settings dialog, under the Controller tab:

1 From the Switch Drivers section, select the switch model from the Model: drop-down options.

○ Off ④	° On						
Controller	Signal Paths Response Correction						
<ul> <li>Autom</li> </ul>	Configuration Mode  Configuration Mode  Automatically select drivers and paths (limited models)  Manually perform these tasks (any supported model)						
Switch Drivers							
Model:	I: BitifEye BIT2100						
Connec	t Keysight U302DA S26 Bitt/Eye BIT2100						

# NOTE

The switch settings and the response correction for all paths are reset if you toggle between switch models.

2 Click the **Connect** button to be able to connect the selected switch driver to a physical switch instrument.

Configu	ure Switch Matrix Settings*	
C Off	• On	
Controller	Signal Paths Response Correction	
<ul> <li>Autor</li> </ul>	ration Mode	
Switch I Model:	Drivers Btt/Eye BIT2100	·]
Conne	ect ID Address / Alias Identification   1 <none> <not connected=""></not></none>	-

- 3 A **Connect to** < *switch-model* > dialog appears, which gives you two options to establish a connection to the selected switch models.
- 4 Select one of the options to establish connection:

#### Enter/Select VISA address/alias (or SICL address)

1 Select **Enter/Select VISA address/alias** to type the complete SICL or VISA address of the switch driver. By default, this option is selected.

Connect to BitifEye BIT2	2100_1 Switch Driver (BitifEye BIT2100_1) ? 🦳 🔀
Currently connected to:	<nothing></nothing>
Change to	
Alias/Address:	USBInstrument1
IDN:	<unknown>Get</unknown>
Enter/Select VISA a	ddress/alias (or SICL address):
USBInstrument1	
Select from Keysight	t Connection Expert 'My Instruments':
	OK Cancel
Ready	

2 Click the **Get** button to identify the instrument at the specified address or alias and to view the current status of the instrument that is connected to the switch driver.

Connect to BitifEye BIT2	2100_1 Switch Driver (BitifEye BIT2100_1) ?	JX.				
Currently connected to: <nothing></nothing>						
Change to						
Alias/Address:	USB0::0x23E0::0x08D2::000024::0::INSTR					
IDN:	BitifEye,BIT2100,000024,3.4.2-1.20 Get					
Enter/Select VISA a	ddress/alias (or SICL address):					
USB0::0x23E0::0x08D	2::000024::0::INSTR	$\mathbf{Y}$				
Select from Keysight	t Connection Expert 'My Instruments':					
	OKCa	ncel				
Ready						

3 Click **OK** to return to the **Configure Switch Matrix Settings** dialog. The connection to the selected switch is displayed.

🖾 Configu	ure Swi	tch Matrix Settings*							
C Off (	⊙ On								
Controller	Controller Signal Paths Response Correction								
Configu	ration N	Node							
<ul> <li>Auton</li> </ul>	maticall	y select drivers and paths (limited models)							
O Manu	ally pe	rform these tasks (any supported model)							
Switch [	Drivers								
Model:		BitifEye BIT2100	-						
Conne	ect	ID Address / Alias Identification							
		1 USB0::0x23E0::0x08D2::000024::0::INSTR BitifEye,BIT2100,000024;3	.4						
	2.2.6.92	III.							
Signal P									
Conne	ection (	Suide							
C Allow	v InfiniS	im for Path Correction							
Connect	Connection Change Actions								
Sleep	Sleep: 0 📩 msec after switches throw								
🗌 Paus	e after (	connection completed (for debug)							
ок		Cancel << Prev Next >> Reset All Save	Load						

4 Click **OK** to save the settings and return to the test environment.

#### Select from Keysight Connection Expert 'My Instruments'

1 Choose **Select from Keysight Connection Expert 'My Instruments'** to control the application with the help of remote PC. Upon selecting this option, the application starts seeking device information from the Keysight Connection Expert.

If remote access of the device is enabled, the **Connect to** *< switch-model >* dialog box displays the list of active instruments.

Connect to BitifEye BIT2100_1 Switch Driver (BitifEye BIT2100_1)									
Currently connected to: <nothing></nothing>									
Change to	Change to								
Alias/Address:	TCPIP0::10.116.33.123::inst0::INST	٤.							
IDN:	<unknown> Get</unknown>								
Enter/Select	VISA address/alias (or SICL address):								
Select from K	Ceysight Connection Expert 'My Instruments':								
📃 Identify / H	Hide unresponsive addresses								
Show SICL	Addresses								
VISA Alias	VISA Address	Manufacturer	Model #	Serial #	Software Version				
	TCPIP0::10.116.33.123::inst0::INSTR	n/a	n/a	n/a	n/a				
USBInstrument1	USBInstrument1 USB0::0x23E0::0x08D2::000024::0::INSTR n/a n/a n/a n/a								
				Re	efresh OK Cancel				
Ready	Ready								

2 Click to select the **Identify / Hide unresponsive addresses** check box to run an IDN query to every instrument in the list and search for the active instruments, if any.

Connect to Biti	fEye BIT2100_1 Switch Driver (BitifEye BIT210	0_1)	_	_	
Currently conne	ected to: <nothing></nothing>				
Change to					
Alias/Address:	TCPIP0::10.116.33.123::inst0::INST	R			
IDN:	<unknown> Get</unknown>				
Enter/Selection	t VISA address/alias (or SICL address):				
O Select from	Keysight Connection Expert 'My Instruments':				
🖌 Identify	/ Hide unresponsive addresses				
Show SI	CL Addresses				
VISA Alias	VISA Address	Manufacturer	Model #	Serial #	Software Version
USBInstrument	t1 USB0::0x23E0::0x08D2::000024::0::INSTF	₹n/a	n/a	n/a	n/a
				Re	fresh OK Cance

3 If any active instruments are found, the **Connect to** <*switch-model*> dialog lists out such instruments. Select the required instrument from the list.



4 Click **OK** to return to the **Configure Switch Matrix Settings** dialog. The connection to the selected switch is displayed.

	ure Switch Matrix Settings*	
○ Off	• On	
Controller	Signal Paths Response Correction	
Autor	ration Mode — natically select drivers and paths (limited models) ally perform these tasks (any supported model)	
Switch	Drivers	
Model:	BitifEye BIT2100	•
Conne	ID Address / Alias Identification USBInstrument1 BtifEye,BIT2100,000024,3.4.2-1.20	

5 Click **OK** in the **Configure Switch Matrix Settings** dialog to save the settings and return to the test environment.



The **Select from Keysight Connection Expert 'My Instruments'** option is available only when the device is powered on and enabled for remote access.

Establishing connection to the Switch Drivers - Manually

The **Manually perform these tasks (any supported model)** option allows you to decide how many drivers to use and how to route the signal paths. It enables the use of any supported switch model.

- In the Configure Switch Matrix Settings dialog:
- 1 Click to select the Manually perform these tasks (any supported model) radio button in the Configuration Mode section.

Configure Switch Matrix Settings*	
○ Off	
Controller Signal Paths Response Correction	
Configuration Mode	
C Automatically select drivers and paths (limited models)	
Manually perform these tasks (any supported model)	

- 2 From the **Switch Drivers** section, select the switch model from the **Model:** drop-down options.
- 3 In the **Switch Drivers** section, you may use the **Add** button to append the list of any additional drivers, which require a connection to an instrument. Use the Delete button to remove a selected driver from the list. Removing the driver from the list dissociates any signal paths that may have been assigned to it earlier.

Configure Switch Matrix Settings*	- C X
C Off C On Controller Signal Paths Response Correction Configuration Mode C Automatically select drivers and paths (limited models) C Manually perform these tasks (any supported model) Switch Drivers	
Model: BttfEye BIT2100	Add Delete
Signal Paths         Use Signal Paths tab to select switch settings.         □ Allow InfiniSim for Path Correction (Reserved for use by application)         Connection Change Actions         □ Sleep:       0         □ Pause after connection completed (for debug)	
OK Cancel << Prev Next >> Reset All Save Load	

4 When you click the **Add**... button, the **Connect**... button appears so that you can establish connectivity to the selected Switch.

🖾 Configur	Switch Matrix Settings*	
⊂ off ⊙	On	
Controller 9	gnal Paths Response Correction	
	on Mode ically select drivers and paths (limited models) y perform these tasks (any supported model)	
Switch Dr	vers	
Model:	BitifEye BIT2100	
Connec	ID   Address / Alias   Identification	Add
	1 <none> <not connected=""></not></none>	Delete
⊂Signal Pa		
Use Signa	ns Paths tab to select switch settings. finiSim for Path Correction (Reserved for use by application)	
Sleep:	n Change Actions 0 msec after switches throw fter connection completed (for debug)	
ОК	Cancel << Prev Next >> Reset All Save Load	

5 The rest of the steps for establishing a connection to the switch model remains the same as described in the previous section. The only difference between automatic and manual modes is that you can add/delete and select switch drivers (any supported model) as per your requirements and preferences in the manual mode.

Configuring Signal Paths

Once you have enabled the Switch Matrix feature and set up connections to the switch drivers, you must configure signal paths. The options to configure the signal paths vary depending upon whether you have selected **Automatically select drivers and paths (limited models)** or **Manually perform these tasks (any supported model)** in the **Controller** tab of the **Configure Switch Matrix Settings** dialog.

Refer to the connection diagram before configuring signal paths either for Automatic or Manual selection. Under the Controller tab, click the **Connection Guide** button to access the Connection Diagram dialog.

Configuring Signal Paths with Automatic Selection

When you have selected **Automatically select drivers and paths (limited models)** in the **Controller** tab of the **Configure Switch Matrix Settings** dialog:

- 1 Click the **Signal Paths** tab. The **Path Assignment** table lists the connection matrix of the device with the Switch modules.
- 2 Scroll down to view the automatic connections that have been established.

At runtime, when the Switch Matrix module is on and when a connection prompt occurs, two events occur:

- The framework suppresses the prompts.
- The Switch Matrix module detects the new connection and then throw switches, as indicated in the Switch column, taking into account the current value of the configuration variable (if any) associated with the connection.

Configuring Signal Paths with Manual Selection

When you have selected **Manually perform these tasks (any supported model)** in the **Controller** tab of the **Configure Switch Matrix Settings** dialog:

- 1 Click the Signal Paths tab in the Configure Switch Matrix Settings dialog.
- 2 Select the channel or switch module in one of the drop-down options. Manually select the alternative channel or driver module from the other drop-down option.
- 3 Optionally, you may change the lane assignments and the corresponding Switch modules.
- 4 Click the **View Connections...** button to view the signal path mapping, to understand how the signal path maps to the connection diagrams being used by the application.
- 5 The **Signal Paths Connection View** dialog is displayed. Select any one of the available options in the **Connection**: drop-down.
- 6 The **Path Assignment & Response Correction** area displays the connections configured for the corresponding connection diagrams in the **Connection:** drop-down.
- 7 Select an entry in the **Path Assignment & Response Correction** area to view the corresponding test information.
- 8 Click the **Tests...** button to view information about the tests that use the selected connection to perform automated tests.
- 9 Click the **Close** button to exit and return to the **Configure Switch Matrix Settings** dialog to finish the signal path configuration.
- 10 If required, use the **Reset Paths...** button to clear all switch and response correction settings for all paths. Click **OK** if you wish to proceed.
- 11 Also, if needed, use the **Load Preconfigured Settings...** button to set switches for all paths as per the recommended settings. Click **OK** if you wish to proceed.

Response Correction

You must specify the response correction after you finish configuring the signal paths. Configuring this area is vital as it impacts the measurement accuracy, credibility and performance of the Oscilloscope. The purpose of response correction is to correct the channel frequency response of the oscilloscope.

Configure	Configure Switch Matrix Settings* —							
○ Off ●	On							
Controller Si	gnal Paths Re	esponse Co	orrection					
Selected P Choose co	ath Actions	None	·	<ctrl> + e)</ctrl>				
<u>E</u> dit S	Settings	E <u>x</u> ecute	e Switches					
Test Point	Driver,Module	e,Switch_Te	erminals in-out	Scope	Response Correction	1		
Lane0+	1,3,1_1-0	ann ann		Channel 1				
Lane1+	1,3,1_2-0			Channel 1				
-								
	h				1			
<u>о</u> к	Cance	<hr/>	< <u>P</u> rev	lext >>	Reset All Sa	ve	Loa	d

For each scope channel that you select, the default response correction method is None, which turns off normalization for the specified path.

You may use the **Edit Settings** button or double-click the selected row to access the corresponding configuration dialog, if you wish to make further changes to a specific scope channel configuration.

Use the **Execute Switches** button to establish a connection between the selected test point and scope channel. The color of this button corresponds to the Oscilloscope Channel where the Switch is connected to.

In the following example, the application displays the prompt indicating that a connection is established when you click **Execute Switches** after selecting the first row. Click **OK** to close the prompt.

100GBASE-CR4 App Test Information	
Path is now connected: [TestPoint Lane0+ ->	Scope Channel 1]
<u>o</u> ĸ	

Once you have finished response corrections for all connections, click **OK** in the **Configure Switch Matrix Settings** dialog. The application redirects you to the test environment.

#### 3 Preparing to Take Measurements

# 4 Main Voltage Measurements

Differential Peak to Peak Output Voltage Test with TX Disabled 41 DC Common Mode Output Voltage Test 42 AC Common Mode Output Voltage Test 43 Differential Peak to Peak Output Voltage Test 44

This section provides the Methods of Implementation (MOIs) for the 100GBASE-CR4 Main Voltage Measurements using a Keysight Infiniium oscilloscope and the 100GBASE-CR4 Test Application.



<b>▼</b> 100G	BASE-CR4 Ap	plication :	100GBASE	-CR4	App Device i	1			X
File Vie	ew Tools He	lp							
Set Up	Select Tests	Configure	Connect	Run	Automate	Results	HTML Report		
SELECT TESTS	<ul> <li>✓ Diffe</li> <li>✓ DC C</li> <li>✓ AC C</li> <li>✓ Diffe</li> <li>Jitter ar</li> <li>Output</li> <li>Return</li> </ul>	oltage Measi rential Peak Common Mo Common Mo rential Peak nd Signaling	to Peak O de Output de Output to Peak O Rate Mea Measureme	Voltag Voltag Voltag output surem ents (p	Voltage Test je Test e Test Voltage Test ents (patter pattern: PRB	: n: PRBS9			
(Click	a test's name	to see its d	escription)						
Message									
<sup>S</sup> 2019-	aries (click for 05-07 01:51:3 05-07 01:51:4	39:812 PM I		ort Ref	reshed	Details ▲ Applic use.	ation initialized	and ready	for
	Uns	saved Chan	ges   4 Tes	ts					

Figure 11 Tests that appear under Main Voltage Measurements

Limits for Main Voltage	The limits for tests under main voltage measurements can be found in section 92.8.3.1 of IEEE 802.3 specifications. Refer to Table 92-6 for corresponding values.
Measurements	• Differential Peak to Peak Output Voltage with TX disabled (max 35 mV)
	DC Common Mode Output Voltage (max 1.9 V)

- AC Common Mode Output Voltage (max 30 mV)
- Differential Peak to Peak Output Voltage (max 1200 mV)

#### Differential Peak to Peak Output Voltage Test with TX Disabled

The purpose of this test is to verify that when TX is disabled the peak-to-peak voltage is less than 35 mV.

**PASS Condition** The max peak-to-peak voltage is less than 35 mV.

**Measurement** 1 Obtain sample or acquire signal data.

- 2 Check that the signal is truly with TX disabled (no valid data transitions).
  - 3 Measure peak-to-peak voltage of the signal.
  - 4 Compare the max peak-to-peak voltage to 35 mV.

# DC Common Mode Output Voltage Test

The purpose of this test is to verify that the common mode signal of the differential pair is between 0-1.9 V.

NOTE	This measurement can be done only with dual-single ended connection; it cannot be done with a differential probing connection.					
PASS Condition	The signal is between 0-1.9 V.					
Measurement Algorithm	<ol> <li>Obtain sample or acquire signal data.</li> <li>Verify that there is a signal and that the connection is dual-single ended.</li> <li>Measure the V<sub>max</sub> and V<sub>min</sub> and get the worst result:</li> </ol>					
	<ul> <li>If the Test Application is running on the DSO Oscilloscope, the Instrument Setup is preset to Real Edge.</li> <li>If the Test Application is running on the UXR Oscilloscope, perform the measurement with the Instrument Setup set to Channels 1 and 2. Repeat the measurement with the Instrument Setup set</li> </ul>					
	to Channels 3 and 4.					

4 Compare the voltage measurement to 0-1.9 V.

#### AC Common Mode Output Voltage Test

The purpose of this test is to verify that the common mode signal of the differential pair rms voltage does not exceed 30 mV.

This measurement can be done only with dual-single ended connection; it cannot be done with a differential probing connection.

PASS Condition The signal is less than 30 mV.

Measurement

NOTE

- 1 Obtain sample or acquire signal data. Algorithm
  - 2 Verify that there is a signal and that the connection is dual-single ended.
  - 3 Measure the V<sub>rms</sub>:
    - · If the Test Application is running on the DSO Oscilloscope, the Instrument Setup is preset to Real Edge.
    - · If the Test Application is running on the UXR Oscilloscope, perform the measurement with the Instrument Setup set to Channels 1 and 2. Repeat the measurement with the Instrument Setup set to Channels 3 and 4.
  - 4 Compare the voltage measurement to 30 mV.

## Differential Peak to Peak Output Voltage Test

The purpose of this test is to verify that the peak-to-peak voltage of the differential signal on a PRBS9 pattern is less than 1200 mV. PASS Condition The differential signal max peak to peak voltage on a PRBS9 pattern is less than 1200 mV. Measurement Obtain sample or acquire signal data. 1 Algorithm

- 2 Verify that there is a signal is connected and has a PRBS9 pattern.
- 3 Measure the peak-to-peak voltage of the differential signal of DUT+ and DUT-.
- 4 Compare the max peak-to-peak voltage to 1200 mV.

# Jitter and Signaling Rate Measurements

Signaling Rate 47 Jitter (Even-Odd Jitter, Bounded Uncorrelated Jitter, Total Uncorrelated Jitter) 48

This section provides the Methods of Implementation (MOIs) for the Jitter and Data Rate Measurements using a Keysight Infinitum oscilloscope and the 100GBASE-CR4 Test Application.



5

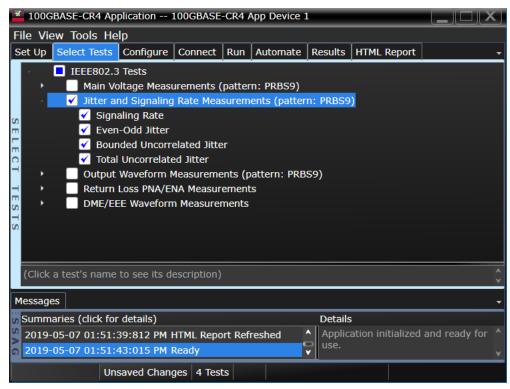


Figure 12 Tests that appear under Jitter and Signaling Rate Measurements

Limits for Jitter and Signaling Rate Measurements The limits for tests under jitter and signaling rate measurements can be found in various sections of IEEE 802.3 specification. Refer to Table 92-6 for corresponding values.

- Signaling Rate (25.78125 ±100 ppm GBd) (section 92.8.3.9)
- Even-Odd Jitter (max 35 mUI) (section 92.8.3.8.1)
- Bounded Uncorrelated Jitter (max 100 mUI) (section 92.8.3.8.2)
- Total Uncorrelated Jitter (max 180 mUI) (section 92.8.3.8.2)

# Signaling Rate

	The purpose of this test is to verify that the signaling rate mean is between 25.78125 $\pm$ 100 ppm G							
PASS Condition	The mean signaling rate is between 25.78125 ±100 ppm GBd.							
Measurement	1 Obtain sample or acquire signal data.							
Algorithm	2 Check that signal is connected and data pattern exists (PRBS9 must be used for this test).							
	3 Set memory depth to capture the number or UI set in the configuration tab.							
	4 Set data rate measurement to semi-automatic 25.78125 Gb/s.							
	5 Measure min, max, mean signaling rate.							
	6 Report min and max values.							

7 Compare and report the mean signaling rate value to 25.78125 ±100 ppm GBd.

Jitter (Even-Odd Jitter, Bounded Uncorrelated Jitter, Total Uncorrelated Jitter)

	The purpose of this test is to verify that differential signal's Even-Odd Jitter is less that 35 mUI, Bounded Uncorrelated Jitter is less than 100 mUI, and Total Uncorrelated Jitter is less than 180 mUI. If all tests are selected, all tests are run on a single measurement. Each test can be run individually by selecting any or some of the tests.
PASS Conditions	<ul> <li>Even-Odd Jitter is less than 35 mUI.</li> <li>Bounded Uncorrelated Jitter is less than 100 mUI.</li> <li>Total Uncorrelated Jitter rms is less than 180 mUI.</li> </ul>
Measurement Algorithm	<ol> <li>Obtain sample or acquire signal data.</li> <li>Check that signal is connected and data pattern exists (PRBS9 must be used for this test).</li> <li>Set memory depth to capture the number or UI set in the configuration tab.</li> <li>Set clock recovery to OJTF First Order PLL with Nominal Data Rate 25.78125 Gb/s and Loop Bandwidth to 10 MHz.</li> </ol>
	5 Using E7 IIT measure Even-Odd litter BUL and TUL at BER of 10E-12

- 5 Using EZJIT, measure Even-Odd Jitter, BUJ, and TUJ at BER of 10E-12.
- 6 Compare and report the values to their respective maximum specification.

# 6

# Output Waveform Measurements

Steady State Voltage Vf 51 Linear Fit Pulse Peak 52 Signal-to-Noise-and-Distortion Ratio 53

This section provides the Methods of Implementation (MOIs) for the Transmitter Output Waveform Measurements for Transition Time using a Keysight Infiniium oscilloscope and the 100GBASE-CR4 Test Application.



₹ 100G	BASE-	CR4 Ap	plication :	100GBASE	-CR4 /	App Device 1			
File Vie	ew To	ols He	lp						
Set Up	Select	: Tests	Configure	Connect	Run	Automate	Results	HTML Report	
	📒 IEE	E802.3	Tests						
•		Main Vo	oltage Measu	urements (	(patter	n: PRBS9)			
•		Jitter a	nd Signaling	Rate Mea	surem	ents (patter	n: PRBS9	)	
- A		Output	Waveform M	Measureme	ents (p	attern: PRB	<mark>59)</mark>		
		🖉 Stea	dy-State Vo	ltage Vf					
		🖉 Linea	ar Fit Pulse I	Peak					
	•	🖉 Sign	al-to-noise-a	and-distor	tion ra	tio			
	•	Norn	nalized Coef	ficient Ste	p Size				
	•	Full	Scale Range	Tests					
•		Return	Loss PNA/EI	NA Measur	rement	S			
· ·		DME/E	E Waveforn	n Measure	ments				
(Click	a test's	s name	to see its d	escription)	)				
lessage	es								
Summ	aries (o	click for	details)				Details	5	
2019-	05-07	01:51:	39:812 PM I	HTML Repo	ort Ref	reshed		ation initialized	and ready for
2019-	05-07	01:51:	43:015 PM I	Ready			■ use.		

Figure 13 Tests that appear under Output Waveform Measurements

Limits for Output Waveform Measurements

- The limits for some tests under output waveform measurements can be found in various sections of IEEE 802.3 specification. Refer to Table 92-6 for corresponding values.
- Steady State Voltage Vf (340-600 mV) (section 92.8.3.5.2)
- Linear Fit Pulse Peak (0.45 \* Vf) (section 92.8.3.5.2)
- Signal-to-noise-and-distortion ratio (26 dB) (section 92.8.3.7)

### Steady State Voltage Vf

Algorithm

The purpose of this test is to verify that the Steady State Voltage as described in section 85.8.3.3 is between 0.34 and 0.6 V.

- **PASS Condition** The Steady State Voltage is between 0.34 and 0.6 V.
  - Measurement 1 Set memory depth to capture one full PRBS9 pattern and scale.
    - 2 Calculate Vf using the equations in section 85.8.3.3.5. The result value is the sum of the columns in P1 (Eq. 85-9).
      - 3 Compare and report the result to 0.34-0.6 V.

#### Linear Fit Pulse Peak

Algorithm

The purpose of this test is to verify that the Linear Fit Pulse as described in section 85.8.3.3 is greater than the Vf \* 0.45.

**PASS Condition** The Linear Fit Pulse is greater than Vf \* 0.45.

#### Measurement 1 Set memory depth to capture one full PRBS9 pattern and scale.

- 2 Calculate p(k) linear fit using the equations in section 85.8.3.3.5. The result value is the max of p(k).
  - 3 Compare and report the result to 0.45\*Vf.

#### Signal-to-Noise-and-Distortion Ratio

The purpose of this test is to verify that the Signal-to-noise-and-distortion ratio (SNDR) is greater than 26dB.

**PASS Condition** The SNDR must be greater than 26dB.

- Measurement<br/>Algorithm1Calculate SNDR using measurements from Level RMS PRBS pattern test and error from Linear<br/>Fit Pulse Peak test.
  - 2 Compare and report the value of SNDR with 26 dB.

#### 6 Output Waveform Measurements

7 Normalized Coefficient Step Size Measurements

abs Coefficient Step Size c(1)inc c(0)hold c(-1)hold57abs Coefficient Step Size c(1)dec c(0)hold c(-1)hold58abs Coefficient Step Size c(1)hold c(0)inc c(-1)hold59abs Coefficient Step Size c(1)hold c(0)dec c(-1)hold60abs Coefficient Step Size c(1)hold c(0)hold c(-1)inc61abs Coefficient Step Size c(1)hold c(0)hold c(-1)inc61

This section provides the Methods of Implementation (MOIs) for the Transmitter Output Waveform Normalized Coefficient Step Size Measurements using a Keysight Infiniium oscilloscope and the 100GBASE-CR4 Test Application.



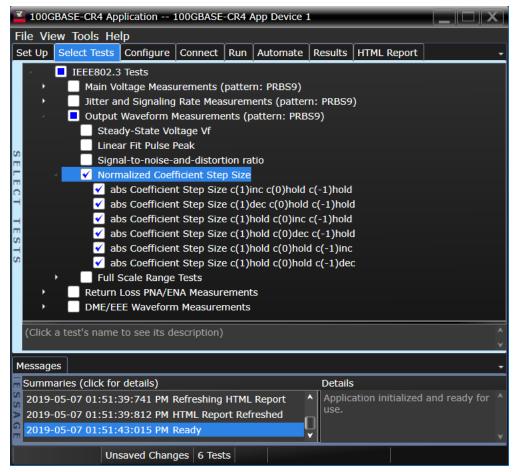


Figure 14 Tests that appear under Normalized Coefficient Step Size

Limits for Normalized Coefficient Step Size Measurements The limits for tests under normalized coefficient step size measurements can be found in various sections of IEEE 802.3 specification. Refer to Table 92-6 for corresponding values.

- abs coefficient step size (min. 0.0083) (section 92.8.3.5.4)
- abs coefficient step size (max. 0.05) (section 92.8.3.5.4)

### abs Coefficient Step Size c(1)inc c(0)hold c(-1)hold

The purpose of this test is to verify that the difference amplitude between coefficient updates falls between the specified values 0.0083 and 0.05.

**PASS Condition** The difference in the coefficient update when c(1) is incremented to the previous is within 0.0083 to 0.05.

#### **Measurement** 1 Request transmitter to be set to 'PRESET' condition.

- $2\quad \text{Set memory depth to capture one full PRBS9 pattern and scale}.$
- 3 Calculate linear fit pulse response at 'PRESET' condition.
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3.
- 5 Request to change the Tx setting to a Baseline condition that allows for increment.
- 6 Calculate the equalized coefficients using equation (85-13).
- 7 Request to change the Tx setting to increment.
- 8 Calculate linear fit pulse response.
- 9 Calculate the equalized coefficients using equation (85-13).
- 10 Compare result to previous setting.
- 11 Loop steps 7-10 for as many increments to be tested.
- 12 Compare and report the values and verify they are in the range of 0.0083 to 0.05.

## abs Coefficient Step Size c(1)dec c(0)hold c(-1)hold

The purpose of this test is to verify that the difference in amplitude between the coefficient updates, falls between the specified values of -0.0083 to -0.05.

**PASS Condition** The difference in the coefficient update when c(1) is decremented to the previous is within -0.0083 to -0.05.

#### **Measurement** 1 Request transmitter to be set to 'PRESET' condition.

- 2 Set memory depth to capture one full PRBS9 pattern and scale.
- 3 Calculate linear fit pulse response at 'PRESET' condition.
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3.
- 5 Request to change the Tx setting to a Baseline condition that allows for decrement.
- 6 Calculate the equalized coefficients using equation (85-13).
- 7 Request to change the Tx setting to decrement.
- 8 Calculate linear fit pulse response.
- 9 Calculate the equalized coefficients using equation (85-13).
- 10 Compare result to previous setting.
- 11 Loop steps 7-10 for as many decrements to be tested.
- 12 Compare and report the values and verify they are in the range of -0.05 to -0.0083.

### abs Coefficient Step Size c(1)hold c(0)inc c(-1)hold

The purpose of this test is to verify that the difference in amplitude between the coefficient updates falls between the specified values of 0.0083 to 0.05.

**PASS Condition** The difference in the coefficient update when c(0) is incremented to the previous state is within 0.0083 to 0.05.

#### **Measurement** 1 Request transmitter to be set to 'PRESET' condition.

- 2 Set memory depth to capture one full PRBS9 pattern and scale.
- 3 Calculate linear fit pulse response at 'PRESET' condition.
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3.
- 5 Request to change the Tx setting to a Baseline condition that allows for increment.
- 6 Calculate the equalized coefficients using equation (85-13).
- 7 Request to change the Tx setting to increment.
- 8 Calculate linear fit pulse response.
- 9 Calculate the equalized coefficients using equation (85-13).
- 10 Compare result to previous setting.
- 11 Loop steps 7-10 for as many increments to be tested.
- 12 Compare and report the values and verify they are in the range of 0.0083 to 0.05.

## abs Coefficient Step Size c(1)hold c(0)dec c(-1)hold

The purpose of this test is to verify that the difference in amplitude between the coefficient updates falls between the specified values of -0.0083 to -0.05.

PASS Condition The difference in the coefficient update when c(0) is decremented to the previous state is within -0.0083 and -0.05.

#### Measurement Request transmitter to be set to 'PRESET' condition. 1

- Algorithm
- 2
- Set memory depth to capture one full PRBS9 pattern and scale. 3 Calculate linear fit pulse response at 'PRESET' condition.
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3.
- 5 Request to change the Tx setting to a Baseline condition that allows for decrement.
- 6 Calculate the equalized coefficients using equation (85-13).
- 7 Request to change the Tx setting to decrement.
- 8 Calculate linear fit pulse response.
- 9 Calculate the equalized coefficients using equation (85-13).
- 10 Compare result to previous setting.
- 11 Loop steps 7-10 for as many decrements to be tested.
- 12 Compare and report the values and verify they are in the range of -0.05 to -0.0083.

### abs Coefficient Step Size c(1)hold c(0)hold c(-1)inc

The purpose of this test is to verify that the difference in amplitude between the coefficient updates falls between the specified values of 0.0083 to 0.05.

PASS Condition The difference in the coefficient update when c(-1) is incremented to the previous state is within 0.0083 and 0.05.

#### Measurement 1 Request transmitter to be set to 'PRESET' condition.

- Algorithm
- 2
- Set memory depth to capture one full PRBS9 pattern and scale. 3 Calculate linear fit pulse response at 'PRESET' condition.
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3.
- 5 Request to change the Tx setting to a Baseline condition that allows for increment.
- 6 Calculate the equalized coefficients using equation (85-13).
- 7 Request to change the Tx setting to increment.
- 8 Calculate linear fit pulse response.
- 9 Calculate the equalized coefficients using equation (85-13).
- 10 Compare result to previous setting.
- 11 Loop steps 7-10 for as many increments to be tested.
- 12 Compare and report the values and verify they are in the range of 0.0083 to 0.05.

## abs Coefficient Step Size c(1)hold c(0)hold c(-1)dec

The purpose of this test is to verify that the difference in amplitude between the coefficient updates falls between the specified values of -0.0083 to -0.05.

**PASS Condition** The difference in the coefficient update when c(-1) is decremented to the previous state is within -0.0083 and -0.05.

#### Measurement 1 Request transmitter to be set to 'PRESET' condition.

- Algorithm
- 2 Set memory depth to capture one full PRBS9 pattern and scale.
- 3 Calculate linear fit pulse response at 'PRESET' condition.
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3.
- 5 Request to change the Tx setting to a Baseline condition that allows for decrement.
- 6 Calculate the equalized coefficients using equation (85-13).
- 7 Request to change the Tx setting to decrement.
- 8 Calculate linear fit pulse response.
- 9 Calculate the equalized coefficients using equation (85-13).
- 10 Compare result to previous setting.
- 11 Loop steps 7-10 for as many decrements to be tested.
- 12 Compare and report the values and verify they are in the range of -0.05 to -0.0083.

# 8 Full Scale Range Tests

Minimum Pre-cursor Full-scale Ratio 65 Minimum Post-cursor Full-scale Ratio 66

This section provides the Methods of Implementation (MOIs) for the Transmitter Output Waveform Full-Scale Range Measurements using a Keysight Infiniium oscilloscope and the 100GBASE-CR4 Test Application.



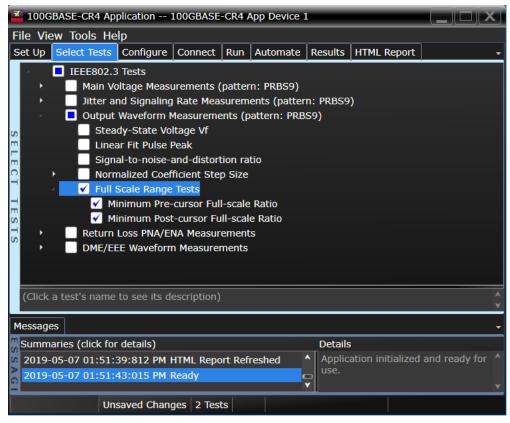


Figure 15 Tests that appear under Full Scale Range Tests

Limits for Full Scale Range Tests The limits for tests under full scale range tests can be found in various sections of IEEE 802.3 specification. Refer to Table 92-6 for corresponding values.

- minimum precursor full-scale ratio (1.54) (section 92.8.3.5.5)
- minimum precursor full-scale ratio (4) (section 92.8.3.5.5)

#### Minimum Pre-cursor Full-scale Ratio

The purpose of this test is to verify that the minimum Pre-cursor is greater than or equal 1.54.

- **PASS Condition** When the coefficients are set to c(1) zero c(0) minimum and c(-1) minimum, the pre-cursor full-scale ratio is greater than or equal 1.54.
  - Measurement Algorithm
- 1 Request transmitter to be set to 'PRESET' condition (only if not previously have 'PRESET' measurement on same trial from step size).
- 2 Set memory depth to capture one full PRBS9 pattern and scale.
- 3 Calculate linear fit pulse response at 'PRESET' condition (if not previously done in same trial on step size).
- 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3 (if not previously done in same trial on step size).
- 5 Request to change the Tx setting to c(-1) zero and c(0) and c(1) to their minimum values.
- 6 Calculate linear fit pulse response.
- 7 Calculate equalized coefficients using equation (85-13).
- 8 Calculate precursor ratio [c(0)-c(-1)]/[c(0)+c(-1)].
- 9 Report and compare the value calculated in step 8 with 1.54.

### Minimum Post-cursor Full-scale Ratio

The purpose of this test is to verify that the minimum Post-cursor is greater than or equal to 4. PASS Condition When the coefficients are set to c(1) minimum c(0) minimum and c(-1) zero, the post-cursor full-scale ration is greater than or equal to 4. Request transmitter to be set to 'PRESET' condition (only if not previously have 'PRESET' Measurement 1 measurement on same trial from step size). Algorithm 2 Set memory depth to capture one full PRBS9 pattern and scale. 3 Calculate linear fit pulse response at 'PRESET' condition (if not previously done in same trial on step size). 4 Define matrix Rm using Equation (92-4) and w using equation (85-2) from IEEE 802.3 (if not previously done in same trial on step size). 5 Request to change the Tx setting to c(1) zero and c(0) and c(-1) to their minimum values. 6 Calculate linear fit pulse response. 7 Calculate equalized coefficients using equation (85-13). 8 Calculate precursor ratio [c(0) - c(1)]/[c(0) + c(1)].

9 Report and compare the value calculated in the previous step with 4.

Keysight D9010BJCC 100GBASE-CR4 Test Application Methods of Implementation

9

# Coefficient Initialization Measurements

Coefficient Initialization (c(0)+c(1)-c(-1))/(c(0)+c(1)+c(-1))69Coefficient Initialization (c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1))70

This section provides the Methods of Implementation (MOIs) for the Transmitter Output Waveform Coefficient Initialization Measurements using a Keysight Infiniium oscilloscope and the 100GBASE-CR4 Test Application.



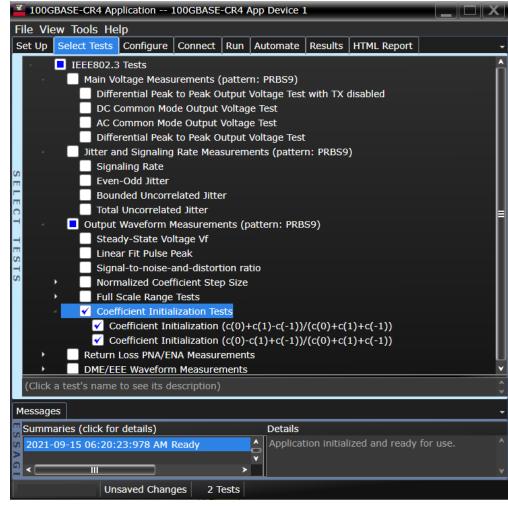


Figure 16 Tests that appear under Normalized Coefficient Step Size

Limits for Coefficient Initialization Measurements The limits for tests under coefficient initialization measurements can be found in section 92.8.3.5.3 of IEEE 802.3-2018 specification.

- Coefficient Initialization (c(0)+c(1)-c(-1))/(c(0)+c(1)+c(-1)) (min. 1.161000 and max.1.419000) (section 92.8.3.5.3)
- Coefficient Initialization (c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1)) (min.2.313000 and max. 2.827000) (section 92.8.3.5.3)

# Coefficient Initialization (c(0)+c(1)-c(-1))/(c(0)+c(1)+c(-1))

	The purpose of this test is to verify that during the PMD (Physical Medium Dependent Sublayer) initialization phase the coefficients of the transmitter equalizer are configured in such a way that the coefficient initialization ratio $(c(0)+c(1)-c(-1))/(c(0)+c(1)+c(-1))$ falls between the specified values.	
PASS Condition	The ratio $(c(0)+c(1)-c(-1))/(c(0)+c(1)+c(-1))$ for coefficients on an initialized signal should fall between 1.161000 and 1.419000.	
Measurement Algorithm	<ol> <li>Request transmitter to be set to 'PRESET' condition (only if there is no existing 'PRESET' measurement on same trial from step size or full scale range tests).</li> </ol>	
	2 Request transmitter to be set to initialize condition.	
	3 Verify that a signal is connected and has PRBS9 pattern.	
	4 Capture the 511 bits of the PRBS9 pattern.	
	5 Calculate the coefficients defined in equation (92-5).	
	6 Calculate the coefficient initialization $(c(0)+c(1)-c(-1)/(c(0)+c(1)+c(-1)))$ based on the results.	

7 Report the result, and verify whether the result is in the range 1.161000 to 1.419000 or not.

#### 9 Coefficient Initialization Measurements

# Coefficient Initialization (c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1))

	The purpose of this test is to verify that during the PMD (Physical Medium Dependent Sublayer) initialization phase the coefficients of the transmitter equalizer are configured in such a way that the coefficient initialization ratio $(c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1))$ falls between the specified values.
PASS Condition	The ratio $(c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1))$ for coefficients on an initialized signal should fall between 2.313000 and 2.827000.
Measurement Algorithm	<ol> <li>Request transmitter to be set to 'PRESET' condition (only if there is no existing 'PRESET' measurement on same trial from step size or full scale range tests).</li> <li>Request transmitter to be set to initialize condition.</li> <li>Verify that a signal is connected and has PRBS9 pattern.</li> <li>Capture the 511 bits of the PRBS9 pattern.</li> <li>Calculate the coefficients defined in equation (92-5).</li> <li>Calculate the coefficient initialization (c(0)-c(1)+c(-1))/(c(0)+c(1)+c(-1)) based on the results.</li> </ol>

7 Report the result, and verify whether the result is in the range 2.313000 and 2.827000 or not.

# 10 Return Loss PNA/ENA Measurements

This section provides the Methods of Implementation (MOIs) for the Return Loss Measurements using a Keysight Infiniium oscilloscope, PNA or ENA, and the 100GBASE-CR4 Test Application. The test application controls the PNA/ENA to set the test limits and run the test. Please ensure that the PNA/ENA are calibrated prior to running a measurement.

#### NOTE

To prevent blank graphs / empty measurement screen-shots being displayed after test run in the HTML Report, it is recommended to use VNC for remotely controlling the PNA/ENA.

PNA - Performance Network Analyzer

ENA - Economy Network Analyzer



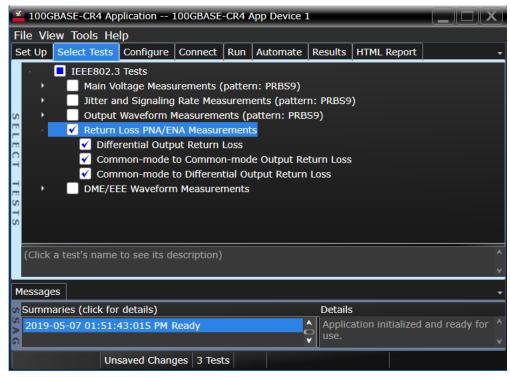


Figure 17 Tests that appear under Return loss PNA/ENA Measurements

Limits for Return Loss PNA/ENA measurements The limits for tests under return loss PNA/ENA measurements can be found in various sections of IEEE 802.3 specification. Refer to Table 92-6 for corresponding values.

- Differential Output Return Loss (refer to section 92.8.3.2 and see Eq. 92-1)
- Common-mode to Common-mode Output Return Loss (refer to section 92.8.3.4 and see Eq. 92-3)
- Common-mode to differential mode Output Return Loss (refer to section 92.8.3.3 and see Eq. 92-2)
- Measurement Algorithm (common for all three tests)
- 1 Ensure that the PNA/ENA is physically connected and calibrated.
- 2 In the **Set Up** tab of the Test Application, click **Connect PNA** or **Connect ENA** to establish connectivity to the connected equipment.
- 3 Click the Select Tests tab and check the tests to measure the Return Loss Measurements.
- 4 Click Run under the Run tab. The Test Application automatically calculates the return loss.
- 5 Compare the reported values with the specification to check for compliance.

Keysight D9010BJCC 100GBASE-CR4 Test Application Methods of Implementation

# 11 DME/EEE Waveform Measurements

DME Differential Peak-to-Peak Output Voltage Test75DME T1-Transition Position Spacing (period) Test76DME T2-Clock Transition to Clock Transition Test77

DME T3-Clock Transition to Data Transition Test 78

EEE Differential Peak-to-Peak Output Voltage Test with TX Disabled 79

EEE Differential Peak-to-Peak Output Voltage Test 80

EEE Common Mode Deviation Voltage Test 81

This section provides the Methods of Implementation (MOIs) for the DME and EEE Waveform Measurements using a Keysight Infinitum oscilloscope and the 100GBASE-CR4 Test Application.



<b>₹</b> 100G	BASE-CR4	Application	100GBASE	-CR4 /	App Device 1		_		x
File Vie	ew Tools	Help							
Set Up	Select Tes	sts Configure	Connect	Run	Automate	Results	HTML Report		
		)2.3 Tests							
		n Voltage Meas							
	=	er and Signaling	-				)		
	Out	put Waveform	Measureme	ents (p	attern: PRB	S9)			
	Reti	urn Loss PNA/E	NA Measur	ement	S				
	🖌 🖌 DME	E/EEE Wavefori	m Measurei	ments					
EO	🗹 D	ME Differentia	Peak to Pe	eak Ou	itput Voltage	e Test			
-	🗹 🗹	ME T1-Transiti	on Position	Spaci	ng (period)	Test			
_	🗹 D	ME T2-Clock T	ransition to	Clock	Transition 1	Test			
m	🗹 D	ME T3-Clock T	ransition to	Data	Transition Te	est			
T	🗹 E	EE Differential	Peak to Pe	ak Ou	tput Voltage	Test with	TX disabled		
S	🗹 E	EE Differential	Peak to Pe	ak Ou	tput Voltage	Test			
	🖌 E	EE Common M	ode Voltag	e Devi	ation Test				
(Click	a test's na	me to see its d	lescription)						
Message	es								
Summ	aries (click	for details)				Details	;		
🧐 2019-	05-07 01:	51:39:812 PM	HTML Repo	ort Ref	reshed	<ul> <li>Applic</li> </ul>	ation initialized	and ready for	
o 2019-	05-07 01:	51:43:015 PM	Ready			⊐ use. ✓			
		Unsaved Chan	ges 7 Tes	ts					

Figure 18

Limits for DME/EEE Waveform measurements The limits for tests under DME/EEE Waveform measurements can be found in various sections of IEEE 802.3 specification. The 100GBASE-CR4 DME specifications can be found in IEEE 802.3ap-2012 section 73.5.1 Table 73-1 and section 73.5.3 Table 73-2. The 100GBASE-CR4 EEE specifications can be found in section 72.7.1 Table 72-6.

- DME Differential Peak-to-Peak Output Voltage (0.6-1.2 V)
- DME T1 (3.2 ns-0.01% to 3.2 ns+0.1%)
- DME T2 (6.2 ns-6.6 ns)
- DME T3 (3.0 ns-3.4 ns)
- EEE Differential Peak-to-Peak Output Voltage with TX disabled (max 30 mV)
- EEE Differential Peak-to-Peak Output Voltage with TX enabled (min 720 mV)
- EEE Common Mode Voltage Deviation (±150 mV)

# DME Differential Peak-to-Peak Output Voltage Test

The purpose of this test is to verify that the peak-to-peak voltage of the differential signal on a 1010 pattern is less than 1200 mV.

**PASS Condition** The differential signal max peak-to-peak voltage on a 1010 pattern is less than 1200 mV.

- Measurement1Obtain sample or acquire signal data.Algorithm2Verify that there is a signal is connect.
  - 2 Verify that there is a signal is connected and has a 1010 pattern.
  - 3 Measure the peak-to-peak voltage of the differential signal of DUT+ and DUT-.
  - 4 Compare the min and max peak-to-peak voltage to be within 0.6 to 1.2 V.

# DME T1-Transition Position Spacing (period) Test

The purpose of this test is to verify that transition spacing of the DME signal is  $3.2 \text{ ns} \pm 0.01\%$ .

PASS Condition	The mean period is between 3.2 ns ±0.01%.
Measurement	1 Obtain sample or acquire signal data.
Algorithm	2 Verify that there is a signal is connected.
	3 Set memory depth to capture the number or UI set in the configuration tab.
	4 Request DUT in DME mode.
	5 Measure the unit interval of the differential DME signal – set UI measurement to SEMI, 3.2e-9.

6 Compare the mean measurement to  $3.2 \text{ ns} \pm 0.01\%$ .

# DME T2-Clock Transition to Clock Transition Test

	The purpose of this test is to verify clock to clock transition is 6.2 ns to 6.6 ns.
PASS Condition	The mean period is between 6.2 ns to 6.6 ns.
Measurement Algorithm	<ol> <li>Obtain sample or acquire signal data.</li> <li>Verify that there is a signal is connected.</li> <li>Set memory depth to capture the number or UI set in the configuration tab.</li> <li>Request DUT in DME mode.</li> <li>Measure the rising to rising edge.</li> </ol>

6 Compare the min and max values to measurement to 6.2 ns to 6.6 ns.

# DME T3-Clock Transition to Data Transition Test

 The purpose of this test is to verify clock to data transition is 3.0 ns to 3.4 ns.

 PASS Condition
 The min and max UI time is between 3.0 ns to 3.4 ns.

 Measurement Algorithm
 1
 Obtain sample or acquire signal data.

 2
 Verify that there is a signal is connected.

 3
 Set memory depth to capture the number or UI set in the configuration tab.

 4
 Request DUT in DME mode.

 5
 Measure the unit interval of the differential DME signal – set UI measurement to SEMI, 3.2e-9.

6 Compare the min and max values to measurement to 3.0 ns to 3.4 ns.

# EEE Differential Peak-to-Peak Output Voltage Test with TX Disabled

The purpose of this test is to verify that when TX is disabled the peak-to-peak voltage is less than 30 mV.

**PASS Condition** The max peak-to-peak voltage is less than 30 mV.

### Measurement Algorithm

- 1 Obtain sample or acquire signal data.
- 2 Request DUT to be EEE mode.
  - 3 Check that the signal is truly with TX disabled (no valid data transitions).
  - 4 Measure peak-to-peak voltage of the signal.
  - 5 Compare the max peak-to-peak voltage to 30 mV.

### 11 DME/EEE Waveform Measurements

# EEE Differential Peak-to-Peak Output Voltage Test

The purpose of this test is to verify that the peak-to-peak voltage of the differential signal on a 1010 pattern is greater or equal to 720 mV.

**PASS Condition** The differential signal max peak-to-peak voltage on a 1010 pattern is greater than or equal to 720 mV.

### **Measurement** 1 Obtain sample or acquire signal data.

- Algorithm 2 F
  - 2 Request DUT in EEE mode.
  - 3 Verify that there is a signal is connected and has a 1010 pattern.
  - 4 Measure the peak-to-peak voltage of the differential signal of DUT+ and DUT-.
  - 5 Compare the min voltage to be greater than or equal to 720 mV.

## EEE Common Mode Deviation Voltage Test

The purpose of this test is to verify that the common mode signal of the differential pair of the pre-LPI signal and the LPI signal is within ±150 mV.

### **PASS Condition** The signal voltage change between pre and post LPI is within 150 mV change.

### Measurement Algorithm

- 1 Obtain sample or acquire signal data.
- 2 Verify that there is a signal and that the connection is dual-single ended.
- 3 Request DUT to be pre-LPI.
- 4 Measure the peak-to-peak voltage.
- If the Test Application is running on the DSO Oscilloscope, the **Instrument Setup** is preset to **Real Edge**.
- If the Test Application is running on the UXR Oscilloscope, perform the measurement with the **Instrument Setup** set to **Channels 1 and 2**. Repeat the measurement with the **Instrument Setup** set to **Channels 3 and 4**.
- 5 Request DUT to be in LPI.
- 6 Measure the peak-to-peak voltage again.
- If the Test Application is running on the DSO Oscilloscope, the **Instrument Setup** is preset to **Real Edge**.
- If the Test Application is running on the UXR Oscilloscope, perform the measurement with the **Instrument Setup** set to **Channels 1 and 2**. Repeat the measurement with the **Instrument Setup** set to **Channels 3 and 4**.
- 7 Calculate Vpp(post)-Vpp(pre).
- 8 Compare the result from step 8 to  $\pm 150$  mV.

### 11 DME/EEE Waveform Measurements

Keysight D9010BJCC 100GBASE-CR4 Test Application Methods of Implementation

# 12 Exporting Measurement Results to Repository

Uploading Results to Repository 84



# Uploading Results to Repository

The Upload Results To Repository feature is an add-on to the Keysight Test Application, where it expands the boundaries of storing and analyzing the measurement results to a wider audience, who may be based in multiple sites across various geographical locations. Along with the feature of exporting test results from the Test Application into your local disk in a CSV or HTML file format, you have the option to upload the test results to a Dataset on a Web Repository. Based on your requirements, you may either upload only a single measurement trial or upload huge volumes of measurement results to any Dataset.

Not only can remote users with an active Internet connection access these Datasets and the corresponding test results on the Web Repository, but they have the option to add and delete Datasets on the Web Server. In the Upload Results To Repository feature, you can even modify the Dataset properties, which are helpful especially when performing a graphical analysis of the uploaded data.

In combination with the *Keysight KS6800A Series Analytics Software*, the Upload Results To Repository feature provides a comprehensive solution to export, view and perform analysis of the measurement results, thereby resulting in qualitative data to ensure that the Device Under Test (DUT) is compliant to the industry standards.

Refer to the *Keysight KS6800A Series Analytics Software Online Help* for more information about the functionality of various features in this software.

To export measurement results to the Repository after the completion of test runs,

- File View Tools Help Connect to Infiniium... t Run Automate Results HTML Report New Project... Open Project... • Save Project Save Project As... Save Project (Settings Only) As... Export Results... CSV User Defined D HTML PDF Print... Print Preview... Repository Page Setup... Exit...
- 1 From the Test Application's main menu, click File > Export Results... > Repository.

The Upload Results to Repository window appears.

2 In the **Connect to Server** pane of the **Datasets** tab, click **Connect...** to login to the Dataset Repository server.

Jpload Re	sults To Repositor	γ	-																																																								
Datasets	Measurements	Properties																																																									
Connect t	o Server ——																																																										
Connect.																																																											
Browse																																																											
Select Da	taset ———																																																										
(Please se	elect one below)																																																										
Select																																																											
Refresh																																																											
Pending Up	bload Summary																																																										
(No measi	urements marked	for upload.)	ŝ.																																																								

3 In the URL: drop-down text field that appears, replace the default text with the actual IP address or the URL along with the port number, if applicable.

You may enter the URL of the Web Repository server, which may be a self-hosted server on your machine (http://localhost:5000/), a remote server or an authentication server. Note that all such URLs accessed via this window appear as a drop-down list in the URL: field.

4 Click the Check button to verify that the KS6800A Series Analytics service is available on the specified web address. Repeat this step each time you edit the web address.

Upload Res	ults To Repositor	γ	2 - IX
Datasets	Measurements	Properties	
Connect to Connect Browse OK Cancel	URL: https://a	ddress:port Check	

- For unrestricted access to the Repository
  - a If the server does not require authentication and the KS6800A Series Analytics service is found on the specified web address, the version information is displayed adjacent to the Check button.

ults To Repositor	у		?   -   X
Measurements	Properties		
o Server ———			ĵ
. URL: http://		:5000/ Check Version 2.0.3	1
	Measurements o Server URL: http://	o Server URL: http://	Measurements Properties o Server URL: http://

- *b* If you click OK, the Upload Results to Repository window displays the connectivity status to the Dataset Repository.
- c Click Browse... to navigate directly to the URL.

Upload Re	sults To Reposito	4	<b>?</b>   <sup>-</sup>  ×
Datasets	Measurements	Properties	
Connect t	o Server ——		
Connecte	d to http://	:5000/	
Connect.			
Browse			

- For restricted access to the Repository
  - a If service is found on the specified URL but access to the web server is restricted based on authentication, the version information is displayed along with the text Authentication Required adjacent to the Check button. Also, the Username: and Password: fields appear. The OK button remains disabled until the authentication credentials are entered.
  - *b* Enter the user credentials in the respective fields, which are required for authentication to access those Datasets that have been created on the web server you are connecting to. For each URL that you access, the Username: drop-down box keeps a record and displays all user names used to access the respective URL.

Upload Res	ults To Repos	itory	
Datasets	Measuremer	nts Properties	
Connect to	o Server —		h
Connect	URL:	http://	
Browse	Username:	LPUser	
	Password:	•••••	
ОК	]		
Cancel	)		J

c Click OK to connect to the entered URL/IP address.

The Connect to Server area displays the connection status along with the username.

d Click Browse... to navigate directly to the URL.

Upload Res	ults To Repositor	у		<b>?</b>  _ ×
Datasets	Measurements	Properties		
Connect t	o Server ——			
Logged in	to: http://		:5000/ as LPUser	
Connect				
Browse				
Logout				

- 5 In the Select Dataset area, click Select... to view the list of Datasets created on the connected repository. Click Refresh to update the list of Datasets that appear in the Test Application's user interface.
- 6 Select the Dataset name where you wish to upload measurement results to. Click OK.

Upload Re	sults To Repository	?   -   ×
Datasets	Measurements Properties	
Connect t	to Server	
Logged in	n to: http://	
Connect.		
Browse		
Logout		
<u></u>		
Select Da	taset	
	C11	
Select	C14	ñ
Refresh	CSV-Import-Test1	
ОК	Example Measurements	
Cancel	eyes	
	Import11	
	JC4	L.
	JSON Import Test1	
	LP1	
	NewDataset1	0.8
	Pareto	×
Pending Up	pload Summary	
	urements marked for upload.)	
		Jpload Close

The Select Dataset area displays the selected Dataset as Active. The Measurements and Properties tabs are enabled after a Dataset is selected.

Upload Results To Repository	
Datasets Measurements Properties	
Connect to Server	
Logged in to: http://www.www.www.www.www.www.www.www.www.w	
Connect	
Browse	
Logout	
Select Dataset	
Active: Example Measurements	
Select	
Refresh	
	إلــــــــــــــــــــــــــــــــــــ
Pending Upload Summary	
(No measurements marked for upload.)	
Uploz	d Close

- 7 Click the **Measurements** tab where the test results from the last test run are displayed.
- 8 You may select and export multiple test results to the repository. You may change the format for the display of measurement data using the drop-down options in the **Group by:** field.

Upload Results To Repository	<b>?</b>
Datasets Measurements Properties	s
Group by: Run Start Time	
Select Run Start Times* to include:	
Run Start Time Run	Duration
2019-03-06 03:19:10:895 00:0	0:22.0210000
<	(Click on a Run Start Time to see measurements.)
*Each row contains results from a sing	gle execution of all checked tests; an N-Times or TestPlan execution
Pending Upload Summary	
(No measurements marked for upload	i.)
	Upload Close

9 After selecting one or more measurements, either click Upload or switch to the Properties tab to associate one or more properties to the measurements that are being uploaded to the Web Server. To perform an enhanced analysis on the measurement data using the *KS6800A Series Analytics Service Software*, Keysight recommends assigning properties to the measurements.

Upload Results To Repository	?   -   X
Datasets Measurements Properties	
Select Properties to Include (Optional):	*
App-Defined —	
Show properties from: O Selected measurements (Additional Info values from Results tab)	
Globals (Settings from Set Up, Configure and HTML Report to	abs)
Auto 🗹 Name Value Type Reported With Name In Repository	
Refresh	
User-Defined	
Add Name Value Type Name In Repository	
Remove	
Pending Upload Summary	
======================================	
Append to Dataset: LPTestData1	
3 measurements from 1 group	
Time stamps will be marked UTC+05:30.	
======================================	
Measurement-reported: 0 of 0 Global: 0 of 27 (Values captured at start of each run)	
Properties will be available in the Results Viewer for splitting and filtering graphs. (Red = Invalid value for type, Orange = Only first 128 characters will be uploaded)	
	oad Close

10 Click the **Properties** tab to assign properties for your measurement results that you select to upload. By default, the **App-Defined** properties are selected to be uploaded in association with the measurement data, wherein only certain aspects of the selected measurements are uploaded. However, you may switch to **Globals** to include as properties one or more options configured under the rest of the tabs of the Compliance Test Application or define one or more custom property values to be associated with the selected measurement data.


Upload Results To Repository								
Datasets Measurements Properties								
Select Properties to Include (Optional):								
App-Defined								
Show properties from:  Selected measurements (Additional Info values from Results tab)								
║ _	Globals	(Settings from Set	: Up, Coi	nfigure and HTML	Report tal	Ľ		
Auto	Name	Value	Туре	Location	Name In			
Refresh	A Hidden Group Config	False	Text	Configure tab	False			
	Clock Channel	Channel 2	Text	Configure tab	False			
	Data Channel	Channel 1	Text	Configure tab	False			
	Debug Mode Used	No	Text	HTML Report ta	b False			
	Debug Only Setting	Default	Text	Configure tab	False	$\ $		
	load Summary					<u>11</u> )		
======								
On web server: http://xxxxxxxxx.cos.is.keysight.com:5000/ Append to Dataset: LPTestData1								
	======================================							
3 measurements from 1 group Time stamps will be marked UTC+05:30.								
======	======================================							
	d properties: ment-reported: 0 of 0							
	of 27 (Values captured at start of )	each run)						
	will be available in the Results View							
(Red = Invalid value for type, Orange = Only first 128 characters will be uploaded)								
Upload Close								

- 11 Click Upload to begin uploading measurement results.
- 12 Click **Close** to exit the **Upload Results to Repository** window and to return to the Compliance Test Application.

You may access the Dataset Repository using the Internet browser on your machine to view the measurement results graphically on the *KS6800A Series Analytics Service Software*.

### KS6800A Series Analytics Service Software

The KS6800A Series Analytics Service software supports multiple data sources and also a wide range of data import clients. This web-based software provides various types of charts, such as Histogram, Box-and-Whisker, Line, Scatter, Eye Diagram and Constellation, each with split capability to enable data analysis. Once you upload the measurement results to a Dataset on the *KS6800A Series Analytics Service Software* via the **Upload Results to Repository** window of the Test Application, the measurement results can be viewed graphically as shown below:

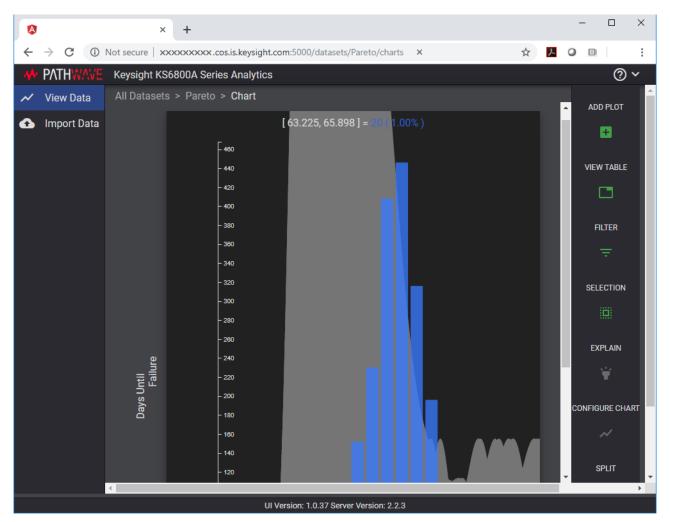

For more information on the Data Analytics Web Service Software, visit KS6800A Series Analytics Service Software page on the Keysight website. You may refer to the Help manual provided within the software to understand the functionality of its features.

Keysight D9010BJCC 100GBASE-CR4 Test Application

Methods of Implementation

# 13 Debug Mode

Debug mode can be selected to make enable the ability to change jitter measurement options. In the **Configuration** tab, select the **Debug** radio button. This will add the following options:

- **Rj Bandwidth** Choose the Rj Filter. Options are Narrow (Pink) or Wide (White). This changes the amount of DC jitter in the Rj measurement.
- Jitter Pattern Length Choose Periodic or Arbitrary. Periodic is used for data patterns that are
  periodic and repeat through the scope memory. Arbitrary is used for random data patterns or long
  data patterns (for example, PRBS31) that do not repeat through the scope memory. If Arbitrary is
  selected, set the ISI filters.
- ISI Filter Lead When using Arbitrary mode for the Jitter Pattern Length, set the Leading ISI filter coefficient. To help select the correct ISI filter, see Application Note 1574: Choosing the ISI Filter Size for EZJIT Plus Arbitrary Data Jitter Analysis (at www.keysight.com, literature part number 5989-4974EN).
- ISI Filter Lag When using Arbitrary mode for the Jitter Pattern Length, set the Lagging ISI filter coefficient. Again, to help select the correct ISI filter, see Application Note 1574: Choosing the ISI Filter Size for EZJIT Plus Arbitrary Data Jitter Analysis.



13 Debug Mode

# Index

# A

- Abs Coefficient Step Size c(1) dec c(0) hold c(-1) hold, 58 Abs Coefficient Step Size c(1) hold c(0) dec c(-1) hold, 60
- Abs Coefficient Step Size c(1) hold c(0) hold c(-1) dec, 62
- Abs Coefficient Step Size c(1) hold c(0) hold c(-1) inc, 61
- Abs Coefficient Step Size c(1) hold c(0) inc c(-1) hold, 59

Abs Coefficient Step Size c(1) inc c(0) hold c(-1) hold, 57

AC Common Mode Output Voltage Test, 43 application software, installing, 12 application software, starting, 19 Automation tab, 22

# В

bounded uncorrelated jitter, 48

# С

calibrating the oscilloscope, 18, 27

# D

data rate, 47 data rate and jitter measurements, 45 DC Common Mode Output Voltage Test, 42 Debug Mode, 93 Differential Peak-to-Peak Output Voltage Test. 44 Differential Peak-to-Peak Output Voltage Test with TX Disabled, 41 DME Differential Peak-to-Peak Output Voltage Test, 75 DME T1-Transition Position Spacing (Period) Test. 76 DME T2-Clock Transition to Clock Transition Test, 77 DME T3-Clock Transition to Data Transition Test, 78

DME/EEE waveform measurements, 73

# Е

EEE Common Mode Deviation Voltage Test, 81
EEE Differential Peak-to-Peak Output Voltage Test, 80
EEE Differential Peak-to-Peak Output Voltage Test with TX Disabled, 79
even-odd jitter, 48

## F

L

full scale range measurements, 63

installation, 7, 11 ISI Filter Lag, 93 ISI Filter Lead, 93

## J

jitter, 48 jitter and data rate measurements, 45 Jitter Pattern Length, 93

## L

license key, installing, 13 Linear Fit Pulse Peak, 52, 53

### Μ

main voltage measurements, 39 main voltage specifications, 40, 46, 50, 56, 64, 68 measurements, preparing, 17 Minimum Post-cursor Full-scale Test, 66 Minimum Pre-cursor Full-scale Test, 65 mouse, 9

# Ν

normalized coefficient step size measurements, 55, 67

# 0

oscilloscope calibration, 18, 27

# R

random jitter, 48 Results tab, 22 return loss ENA/PNA measurements, 71 Rj Bandwidth, 93 Run Tests tab, 22

# S

Set Up tab, 21 specifications, main voltage, 40, 46, 50, 56, 64, 68 specifications, transmitter output, 46, 50, 56, 64, 68 Steady State Voltage Vf, 51

# Т

transmitter output specifications, 46, 50, 56, 64, 68 transmitter output waveform measurements, 49 Index