

Keysight 8472B Crystal Detector

Notices

Copyright Notice

© Keysight Technologies 2014 - 2019

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies as governed by United States and international copyright laws.

Manual Part Number

08472-90022

Edition

Edition 2, January 10, 2019

Printed in:

Printed in Malaysia

Published by:

Keysight Technologies
Bayan Lepas Free Industrial Zone,
11900 Penang, Malaysia

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Declaration of Conformity

Declarations of Conformity for this product and for other Keysight products may be downloaded from the Web. Go to <http://www.keysight.com/go/conformity>. You can then search by product number to find the latest Declaration of Conformity.

U.S. Government Rights

The Software is "commercial computer software," as defined by Federal Acquisition Regulation ("FAR") 2.101. Pursuant to FAR 12.212 and 27.405-3 and Department of Defense FAR Supplement ("DFARS") 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public. Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at <http://www.keysight.com/find/sweula>. The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight: (1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release, perform, display, or disclose commercial computer software or commercial computer software documentation. No additional government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no greater than Limited Rights as defined in FAR 27.401 or DFAR 227.7103-5 (c), as applicable in any technical data.

Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED, WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR OF ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT SHALL CONTROL.

Safety Information

CAUTION







A CAUTION notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING



A WARNING notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Safety Symbols

The following symbols on the instrument and in the documentation indicate precautions which must be taken to maintain safe operation of the instrument.

	<p>When you see this symbol on your instrument, you should refer to the instrument's instruction manual for important information.</p>		<p>This symbol indicates hazardous voltages.</p>
	<p>The laser radiation symbol is marked on products that have a laser output.</p>		<p>This symbol indicates that the instrument requires alternating current (ac) input.</p>
	<p>This symbol indicates that the power line switch is ON.</p>		<p>This symbol indicates that the power line switch is OFF or in STANDBY position.</p>

Regulatory Markings

	<p>The CE mark is a registered trademark of the European Community. This CE mark shows that the product complies with all the relevant European Legal Directives.</p>		<p>The CSA mark is a registered trademark of the Canadian Standards Association.</p>
<p>ISM 1-A</p>	<p>This text indicates that the instrument is an Industrial Scientific and Medical Group 1 Class A product (CISPER 11, Clause 4).</p>		

Waste Electrical and Electronic Equipment (WEEE) Directive

This instrument complies with the WEEE Directive marking requirement. This affixed product label indicates that you must not discard this electrical or electronic product in domestic household waste.

Product category:

With reference to the equipment types in the WEEE directive Annex 1, this instrument is classified as a “Monitoring and Control Instrument” product.

The affixed product label is as shown below.



Do not dispose in domestic household waste.

To return this unwanted instrument, contact your nearest Keysight Service Center, or visit <http://about.keysight.com/en/companyinfo/environment/takeback.shtml> for more information.

Sales and Technical Support

To contact Keysight for sales and technical support, refer to the support links on the following Keysight websites:

- www.keysight.com/find/adapters
(product-specific information and support, software and documentation updates)
- www.keysight.com/find/assist
(worldwide contact information for repair and service)

Table of Contents

Safety Symbols	3
Regulatory Markings	3
.....	3
Waste Electrical and Electronic Equipment (WEEE) Directive	4
Product category:	4
Sales and Technical Support	4
List of Figures	7
List of Tables	9
Description	11
Installation	12
Initial inspection	12
Storage and shipment	12
Specifications	13
Operating Information	15
Operator's checks	16
Performance Tests	18
Frequency response test	18
Higher level sensitivity test	18
Low level sensitivity test	18
Match test (SWR)	18
Service Instructions	19
Repair and replacement	19

THIS PAGE HAS BEEN INTENTIONALLY LEFT BLANK.

List of Figures

Figure 1	Peak power measurement	16
----------	------------------------------	----

THIS PAGE HAS BEEN INTENTIONALLY LEFT BLANK.

List of Tables

Table 1	Specifications	13
---------	----------------------	----

THIS PAGE HAS BEEN INTENTIONALLY LEFT BLANK.

Description

The 8472B crystal detector is a 50 Ω (nominal) device designed for measurement use in coaxial systems.

Features

- The instrument converts RF power levels applied to the 50 Ω input connector into proportional values of DC voltage.
- The instrument measures relative power up to 200 mW and has a BNC female connector for the output jack which allows the detected output to be connected to a SWR meter.
- The output voltage polarity is negative, unless Option 003 is selected.
- The frequency range of the detector is 10 MHz to 18 GHz.

Options

The 8472B crystal detector is available with the following options. Refer to [Table 1](#) for further descriptions.

Option 001: Matched pair of detectors

Option 002: Optimum square law load

Option 003: Positive polarity output

Option 100: Female OSSM type output connector

Mating connectors

- The mating output connector used with the crystal detector must be a male BNC connector for the standard output connector or an OSSM male connector for Option 100.
- The mating RF input connector must be a female SMA connector.

CAUTION

SMA connectors have a limited life in applications that require repeated connecting and disconnecting. In-series adapters should be used for such applications.

Installation

Initial inspection

- 1** Inspect the shipping container for damage. If the shipping container or cushioning material is damaged, it should be kept until the contents of the shipment have been checked for completeness and the instrument has been checked mechanically and electrically. Procedures for checking electrical performance are given under Performance Tests.
- 2** If the contents are incomplete, if there is mechanical damage or defect, or if the instrument does not pass the electrical performance test, contact the nearest Keysight Technologies office. Refer to “Sales and Technical Support” on page 4. Keysight Technologies will arrange for repair or replacement of the damaged or defective equipment. Keep the shipping materials for the carrier’s inspection.
- 3** If you are returning the instrument for service, repackaging the instrument requires original shipping containers and materials or their equivalents. Keysight Technologies can provide packaging materials identical to the original materials. Refer to “Sales and Technical Support” on page 4. Attach a tag indicating the type of service required, return address, model number and serial number. Mark the container **FRAGILE** to insure careful handling. In any correspondence, refer to the instrument by model number and serial number.

Storage and shipment

The instrument should be stored in a clean, dry environment. The following environmental limitations apply to both storage and shipment:

- a** Temperature: -54 C to +85 °C
- b** Altitude: < 7620 meters (25,000 feet)
- c** Humidity: < 95% relative
- d** Shock: 100 G for 11 ms
- e** Vibration: 20 G from 80 to 2000 Hz

Specifications

Specifications are performance standards or limits against which the detectors are tested.

Table 1 Specifications

Characteristic	Value
Frequency range ^[a]	10 MHz to 12.4 GHz
Frequency response ^{[b][c][e]}	
Octave flatness	±0.2 dB over any octave 10 MHz to 8 GHz
Broadband flatness	±0.3 dB 10 MHz to 12.4 GHz ±0.5 dB 10 MHz to 15 GHz ±0.6 dB 10 MHz to 18 GHz
SWR ^{[b][c]} (max)	10 MHz to 4.5 GHz, 1.2 4.5 GHz to 7.0 GHz, 1.35 7.0 GHz to 12.4 GHz, 1.50 12.4 GHz to 18 GHz, 1.70
Maximum operating input power	200 mW, peak or average
Maximum short term input power	1 watt (typical) peak or average for < 1 minute
Sensitivity ^{[b][d][e]}	
High level	< 0.35 mW produces 100 mV output
Low level	> 0.5 mVdc/μW CW
Input impedance	50 Ω (nominal)
Output impedance	1 to 2 kΩ (typically 1.3 kΩ) shunted by 40 to 60 pF (typically 50 pF).
Output polarity	Negative (refer to Options for positive polarity units)
Detector element	Supplied (refer to “Repair and replacement” on page 19)
Bias	Not required
Noise	< 50 mVpp with CW applied to produce 100 mV output, 400 kHz bandwidth.
Options	
Option 001	Matched detector pair. Frequency response characteristics (exclusive of basic sensitivity) track within ±0.2 dB from 10 MHz to 12.4 GHz, ±0.3 dB from 12.4 GHz to 18 GHz.
Option 002	Furnished with matched load resistor for optimum square law characteristics of 25 °C, within ±0.5 dB from square law over a range of at least 30 dB up to 10 mV peak output, working into an external load > 8 k W. Sensitivity typically is greater than 0.1 mV/mW when load resistor is used.
Option 003	Positive polarity output
Option 100	Female OSSM-type output connector

Table 1 Specifications (continued)

Characteristic	Value
Environmental	
Operating temperature	-20°C to +85 °C
Humidity	< 95% relative
Vibration	20 G from 80 to 2000 Hz
Shock	100 G for 11 ms
Altitude	< 4570 meters (15,000 feet)
General	
Weight	Net 114 g (4 oz.)
Dimensions	64 mm long, 19mm diameter (2.50 in. long, 0.75 in.diameter)

[a] RF may leak through the output connector below 1 GHz. It can be reduced, if objectionable, with a suitable low pass filter.

[b] Specifications given for +25 °C unless otherwise noted.

[c] Measurement made at -20 dBm.

[d] Sensitivity decreases with increasing temperature, typically:
 0.5 dB from -20 to +25 °C;
 0.5 dB from +25 to +40 °C;
 1 dB from +40 to +55 °C;
 1.25 dB from +55 to +75 °C;
 1 dB from +75 to +85 °C.

[e] External load resistance > 50 k Ω

Operating Information

The crystal detector can be used as a demodulator to obtain a pulse envelope which can then be observed on an oscilloscope. It can also be used as a general purpose detector.

CAUTION

- Static discharge can damage the detector element. A 100 pF capacitor (1.2 m [4 ft] of coax cable) charged to 14 volts stores .1 erg, the maximum pulse rating of the detector element.
 - Connect cables to test equipment and discharge the center conductor before you connect to the detector.
 - **DO NOT NEEDLESSLY HANDLE THE DETECTOR ELEMENT USED IN CRYSTAL DETECTOR.** Static electricity which builds up on a person, especially on a cold dry day, must never be allowed to discharge through the crystal detector.
 - Avoid exposed leads to or from the crystal detector, since these are often touched accidentally.
-

The power applied to the detector can be either modulated or continuous wave (CW). If modulated at a 1000 Hz rate, a SWR meter can be used as an indicator. For CW detection, a DC milliammeter or millivoltmeter can be used as the indicator.

NOTE

When using the crystal detector with an oscilloscope, and the waveshapes to be observed have rise times of less than 5 μ s, the coaxial cable connecting oscilloscope and detector should be as short as possible and shunted with a resistor.

Ideally, this resistor should be 50 Ω to terminate the coaxial cable properly. However, with 50 Ω resistance, the output video pulse may be too small to drive some oscilloscopes. Therefore, the cable should be shunted with the smallest value of resistance that will obtain suitable deflection on the oscilloscope; typically the value will lie between 50 Ω and 2 k Ω . The larger the resistance, the more degradation of rise time.

Operator's checks

Peak power measurement

The procedure for peak power measurement involves calibration of an oscilloscope which, in turn, is used to calibrate a CW generator. The output of the calibrated CW generator is measured with a power meter and thereby the peak power of a pulse is measured.

Refer to **Figure 1** for the equipment setup in the steps referenced below.

- 1 Measure the output amplitude resulting from the pulse.
 - a Connect equipment as shown in **Figure 1**, step A.
 - b Observe the pulse on a de-coupled oscilloscope.
 - c Using a marking pencil, mark on the graticule the base-to-peak amplitude of the pulse envelope.
- 2 Match the output amplitude to the CW source power.
 - a Replace the pulse source with a CW generator.
 - b While observing the oscilloscope trace, adjust the amplitude of CW generator output to make the detector's output equal to that of the pulse generator, as indicated by markings on the graticule (step A).
- 3 Measure the output power from the CW source.
 - a Leave the CW generator at the setting obtained in step B.
 - b Disconnect the detector from CW generator.
 - c Connect the output of CW generator to the power meter (step C).
 - d Measure the adjusted levels (set in step B) of the CW generator output. The peak power of the pulse envelope observed in step A is equal to the output power of the CW generator.

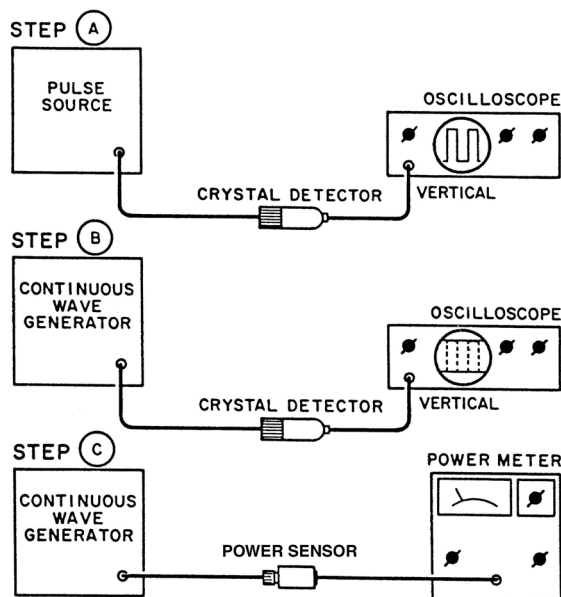


Figure 1 Peak power measurement

Reflectometer application

For information about reflectometer systems and measurements refer to the *Keysight Technologies Application Note Index*. Copies are available upon request.

Harmony frequency comparison measurement application

The detector can be used as a mixer in harmonic-frequency comparison measurements. Refer to the *Keysight Technologies Application Note Index* for further information.

Performance Tests

Methods for testing detector specifications are given below. Refer to the manuals of the equipment involved for specific operating instructions.

NOTE

Multiple mismatch errors caused by attenuator SWR, power meter SWR, and detector SWR should be taken into account, as well as the accuracy of the indicator used to measure the detector's output.

Frequency response test

- 1 Using signal sources covering 10 MHz to 18 GHz with a 10 dB isolating attenuator and a power meter, connect the power sensor to the attenuator. Adjust the CW RF power level to -20 dBm input to the power sensor.
- 2 Without changing the RF power level of signal source, disconnect the power sensor.
- 3 Connect the detector to the attenuator. Measure the DC voltage output and record the measurement.
- 4 Change the frequency of the signal source and repeat steps 1 through 3.
- 5 Since the detector follows a square-law response at this power level, its output is proportional to power ($P_{dB} = 10 \log V_o$). Total variation of detector readings should meet specifications (refer to [Table 1](#)) for all frequencies of interest across the band.

Higher level sensitivity test

- 1 Using signal sources covering 10 MHz to 18 GHz and a DC voltmeter or oscilloscope as the indicator, connect the detector to the signal source. Adjust the RF power level for a 100 mV detected output from the detector, using a CW signal.
- 2 Disconnect the detector from the signal source and measure the RF output level. The RF output level should be ≤ 0.35 mW.
- 3 Repeat steps 1 and 2 for all frequencies of interest across the band.

Low level sensitivity test

- 1 Using a signal source (covering 10 MHz to 18 GHz), a 10 dB attenuator, and a power meter, connect the attenuator to the signal source and power sensor to the attenuator. Adjust the RF power level for -20 dBm output from the attenuator. Verify the ambient temperature.
- 2 Disconnect the power sensor from the attenuator and connect the detector. Measure the DC voltage output from the detector. The output should be > 5.0 mV at 25°C . Between 20°C and 30°C the sensitivity slope is typically -0.04 dB/ $^\circ\text{C}$.

Match test (SWR)

- 1 To verify the detector's SWR specifications, use any system whose measurement accuracies for SWR (residual SWR) are known.

Service Instructions

Repair and replacement

For repair and replacement information or any other additional maintenance information, refer to **“Sales and Technical Support”** on page 4 for the nearest Keysight Technologies Sales and Service office.

The detectors have no internal adjustments.

THIS PAGE HAS BEEN INTENTIONALLY LEFT BLANK.



This information is subject to change without notice. Always refer to the Keysight website for the latest revision.

© Keysight Technologies 2014 - 2018
Edition 2, December 10, 2018

Printed in Malaysia



08472-90022

www.keysight.com